


FIG. 1

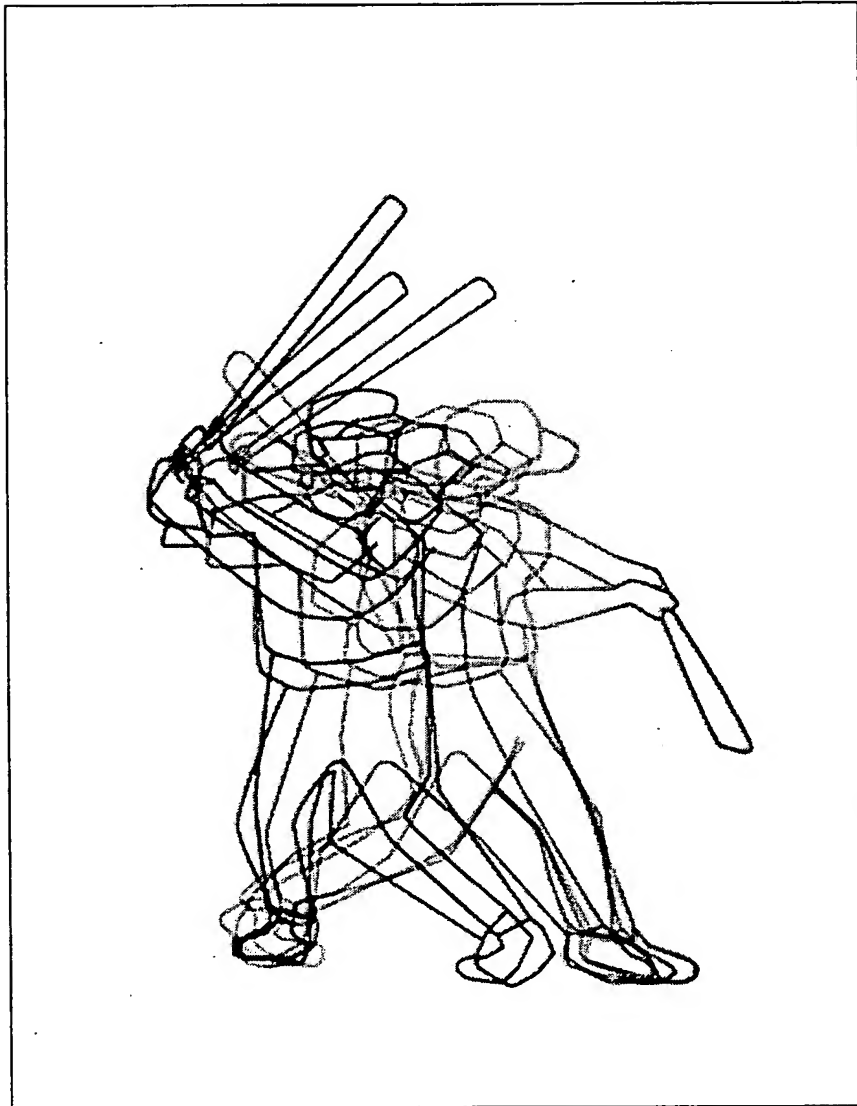

BEST AVAILABLE COPY

FIG. 2

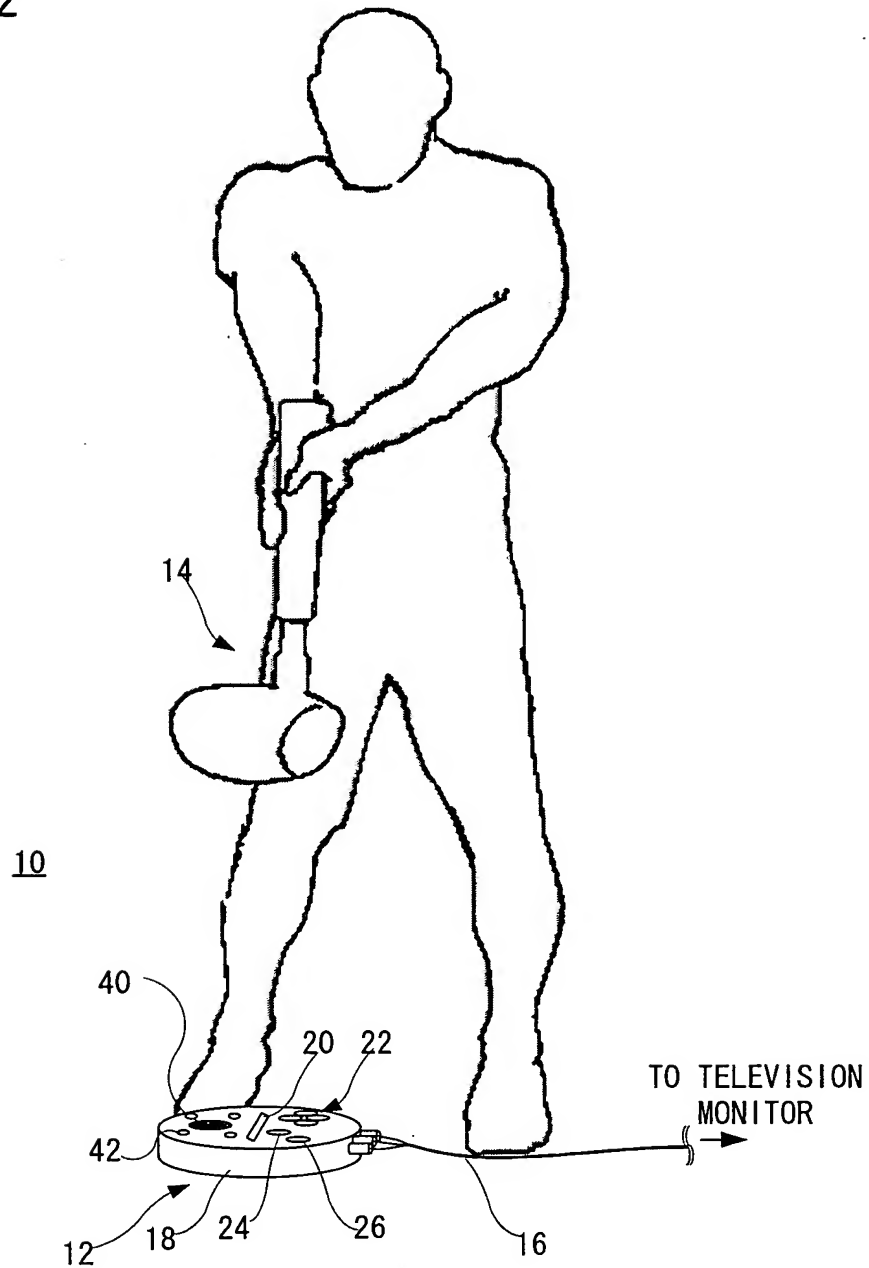


FIG. 3

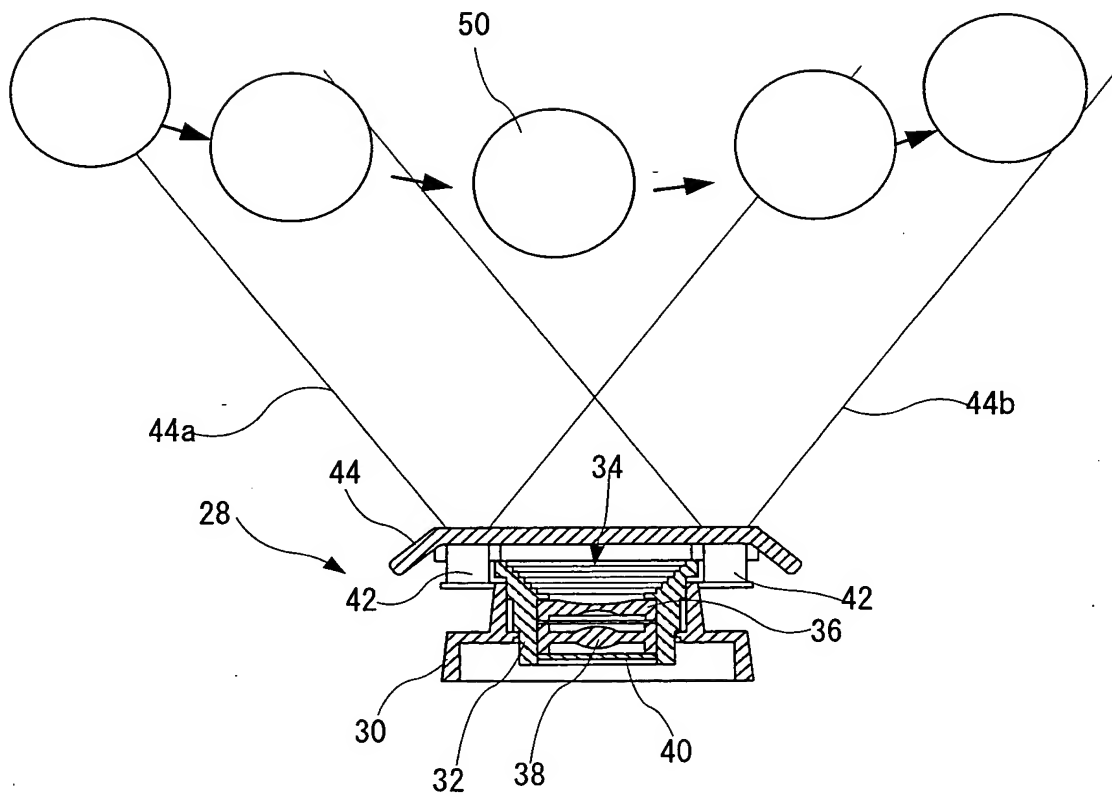


FIG. 4

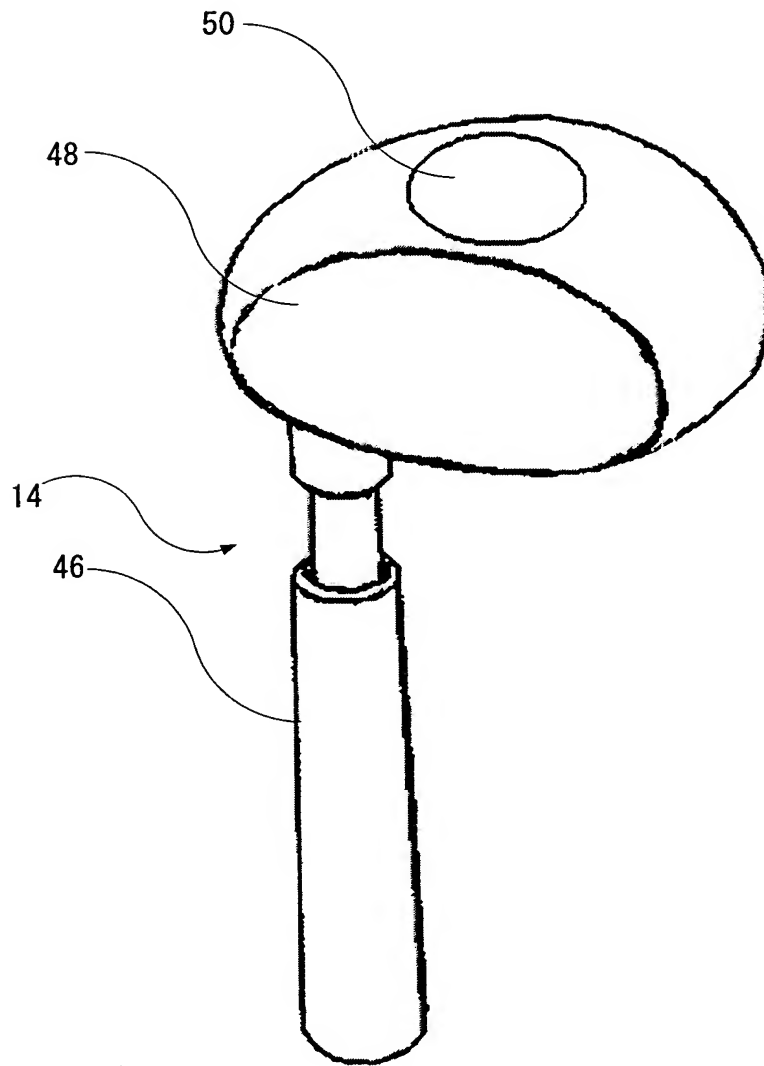


FIG. 5

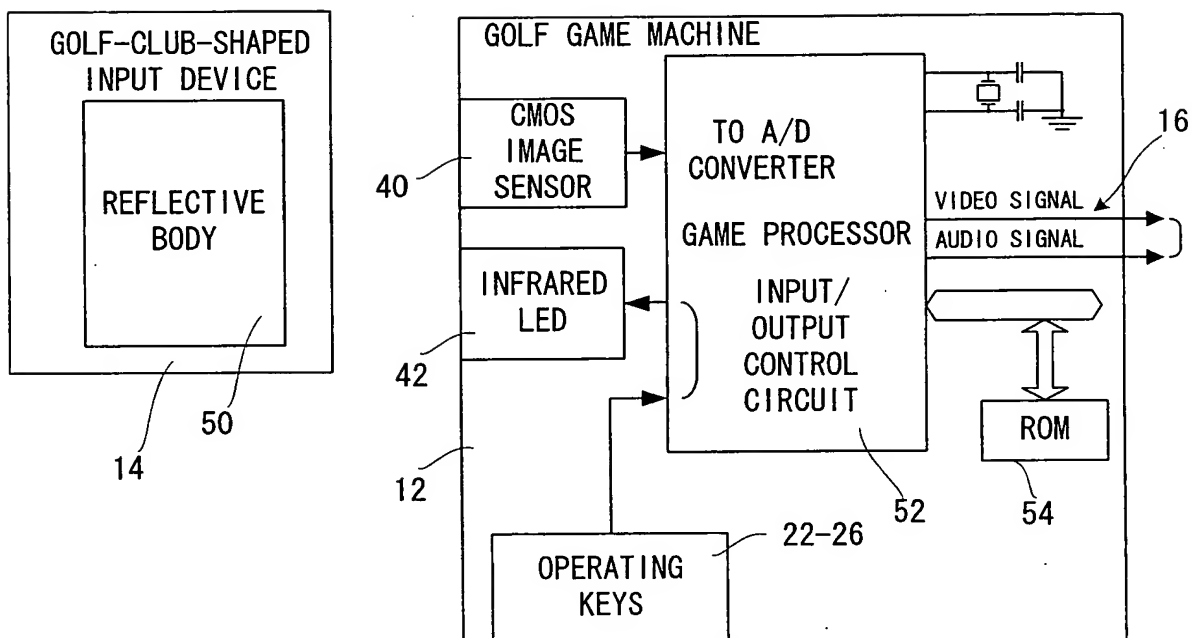


FIG. 6

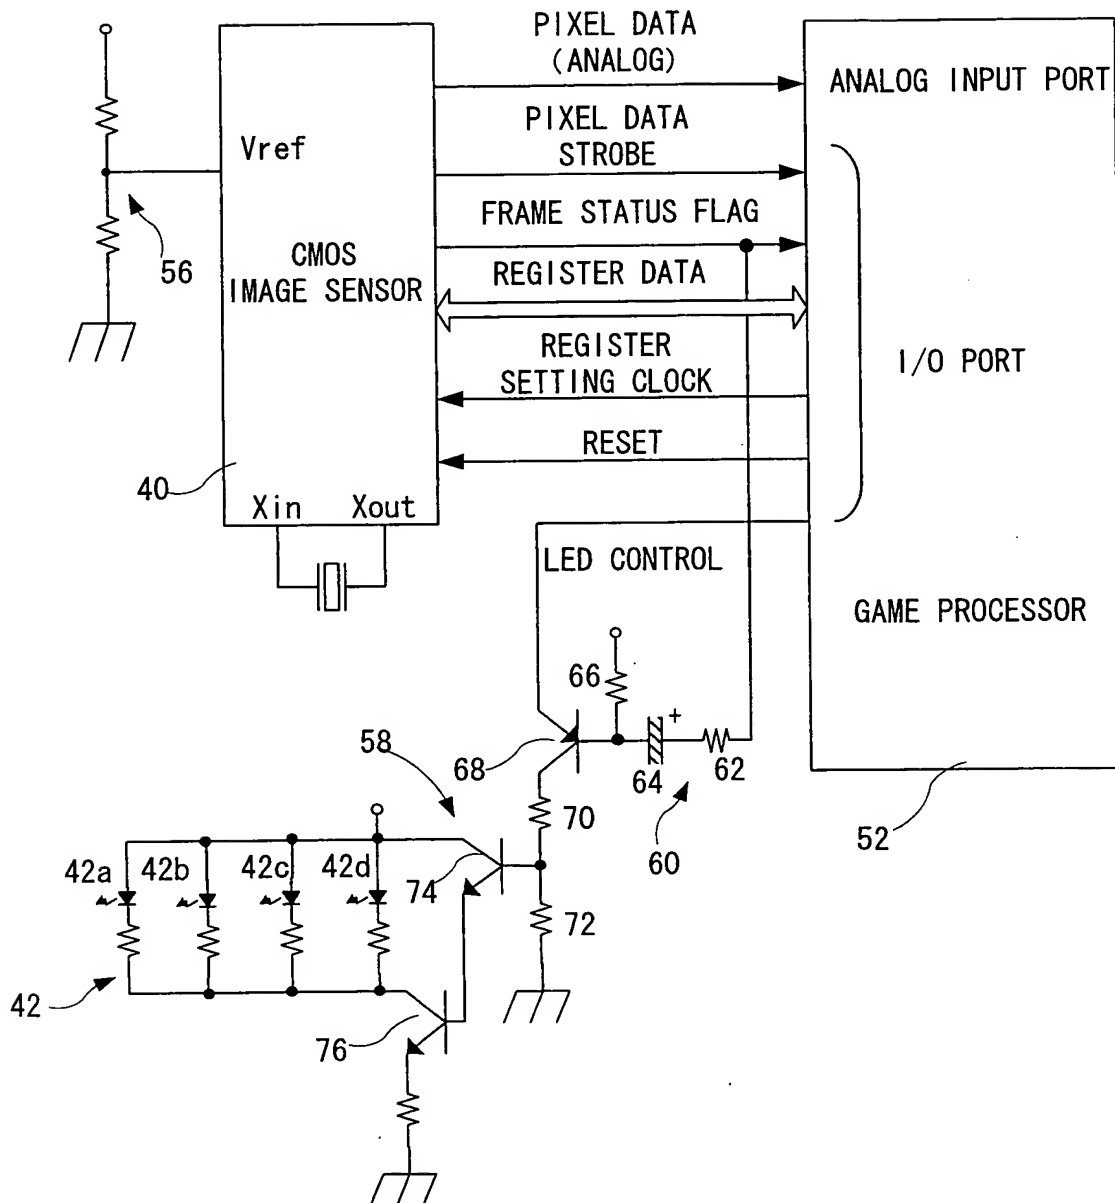


FIG. 7

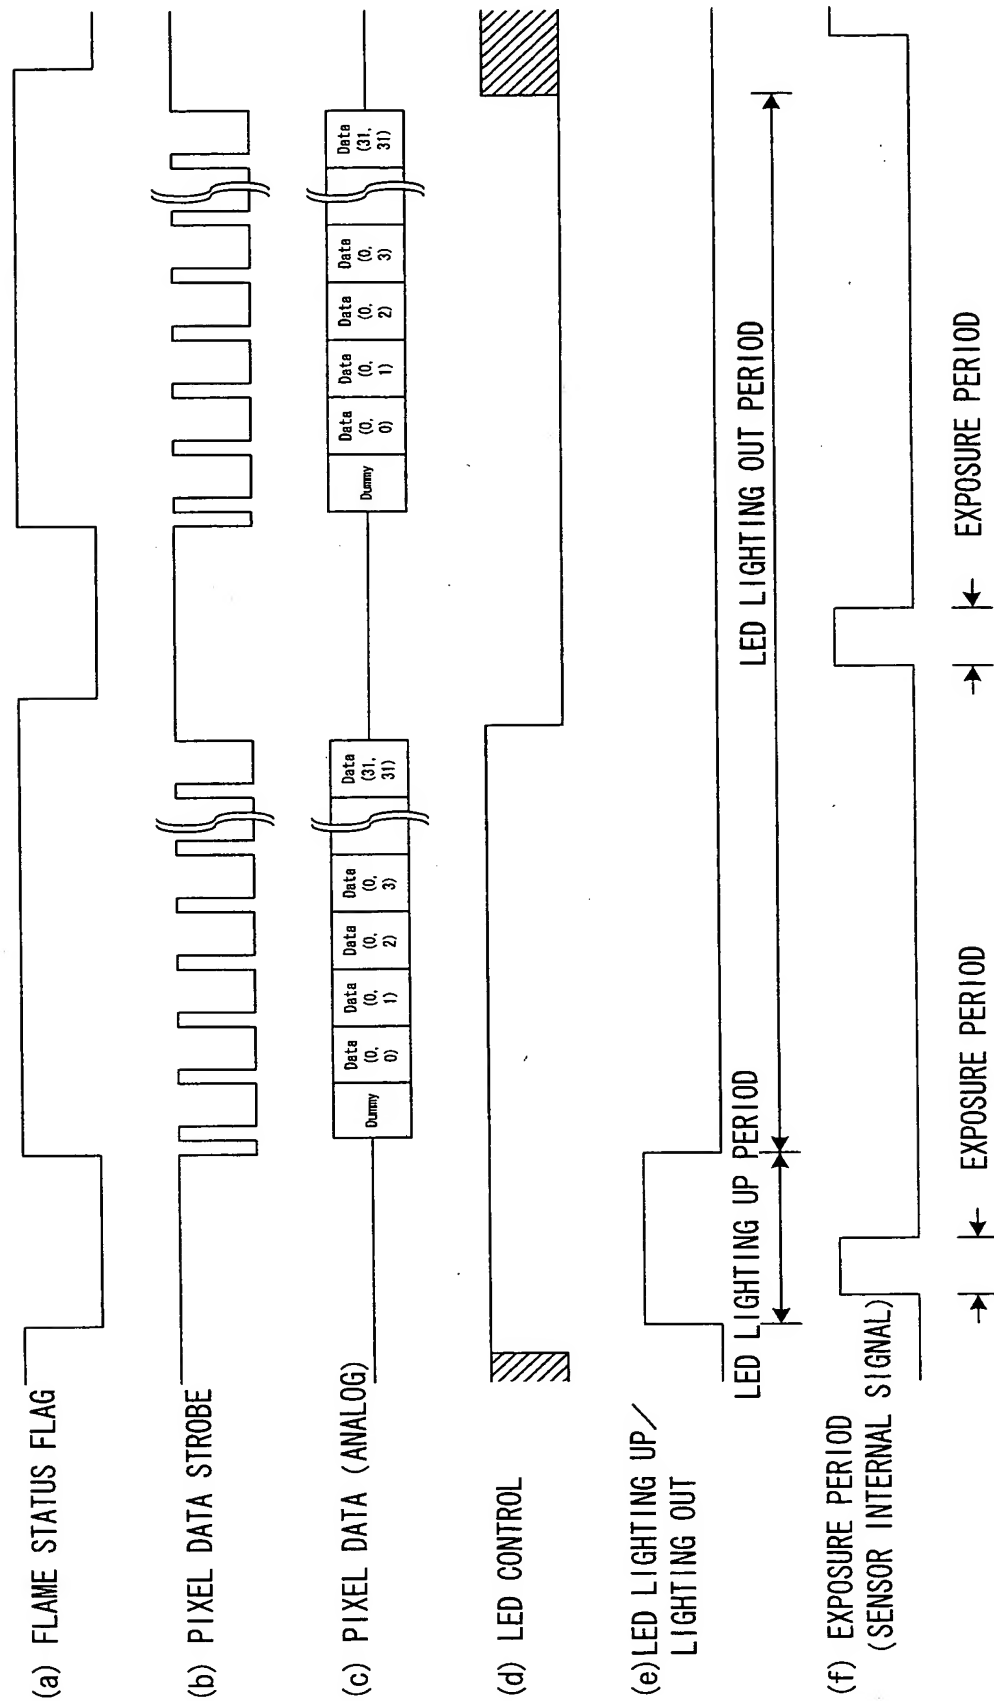


FIG. 8

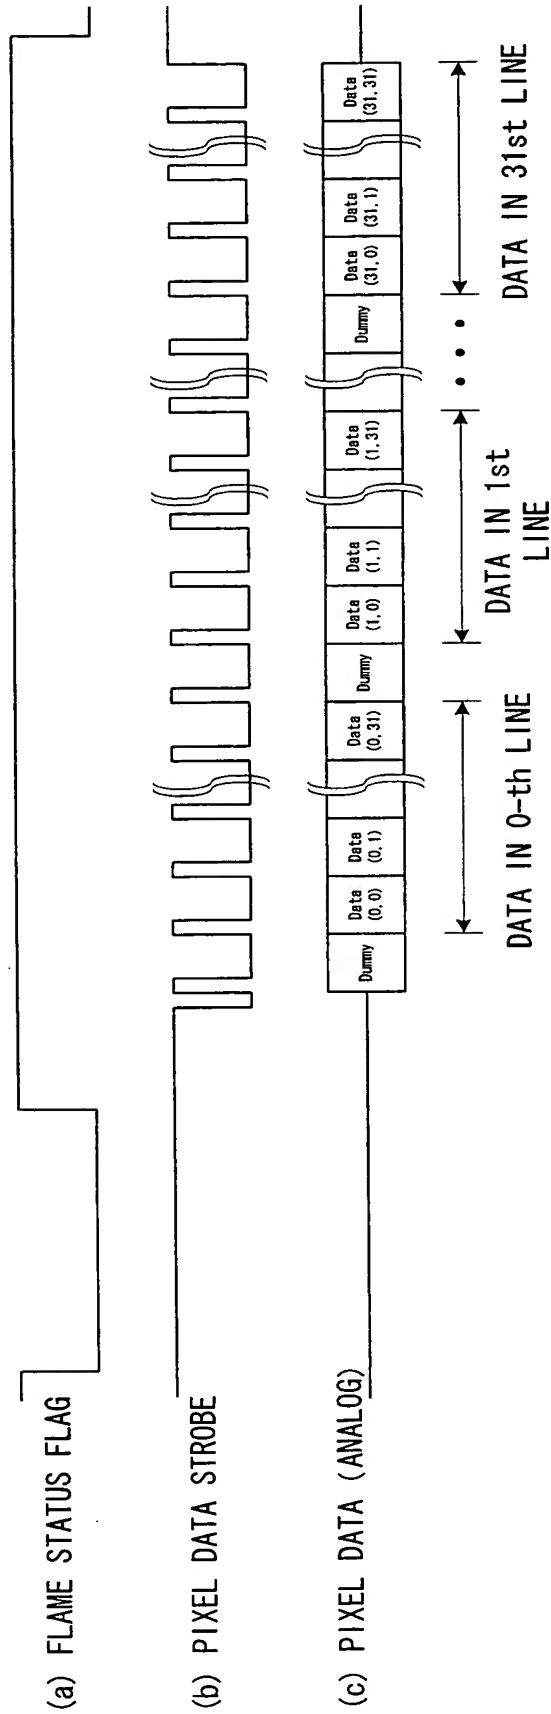


FIG. 9

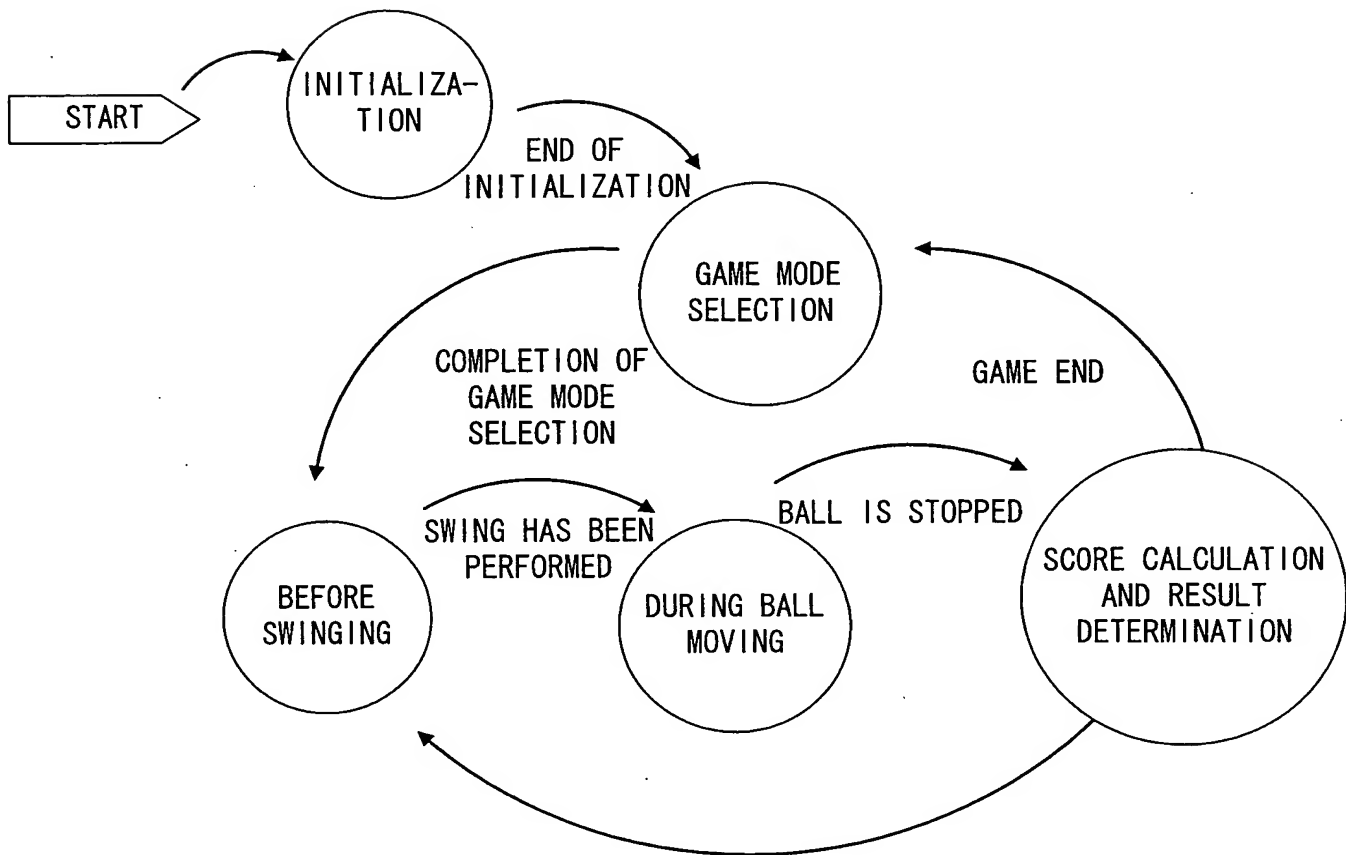


FIG. 10

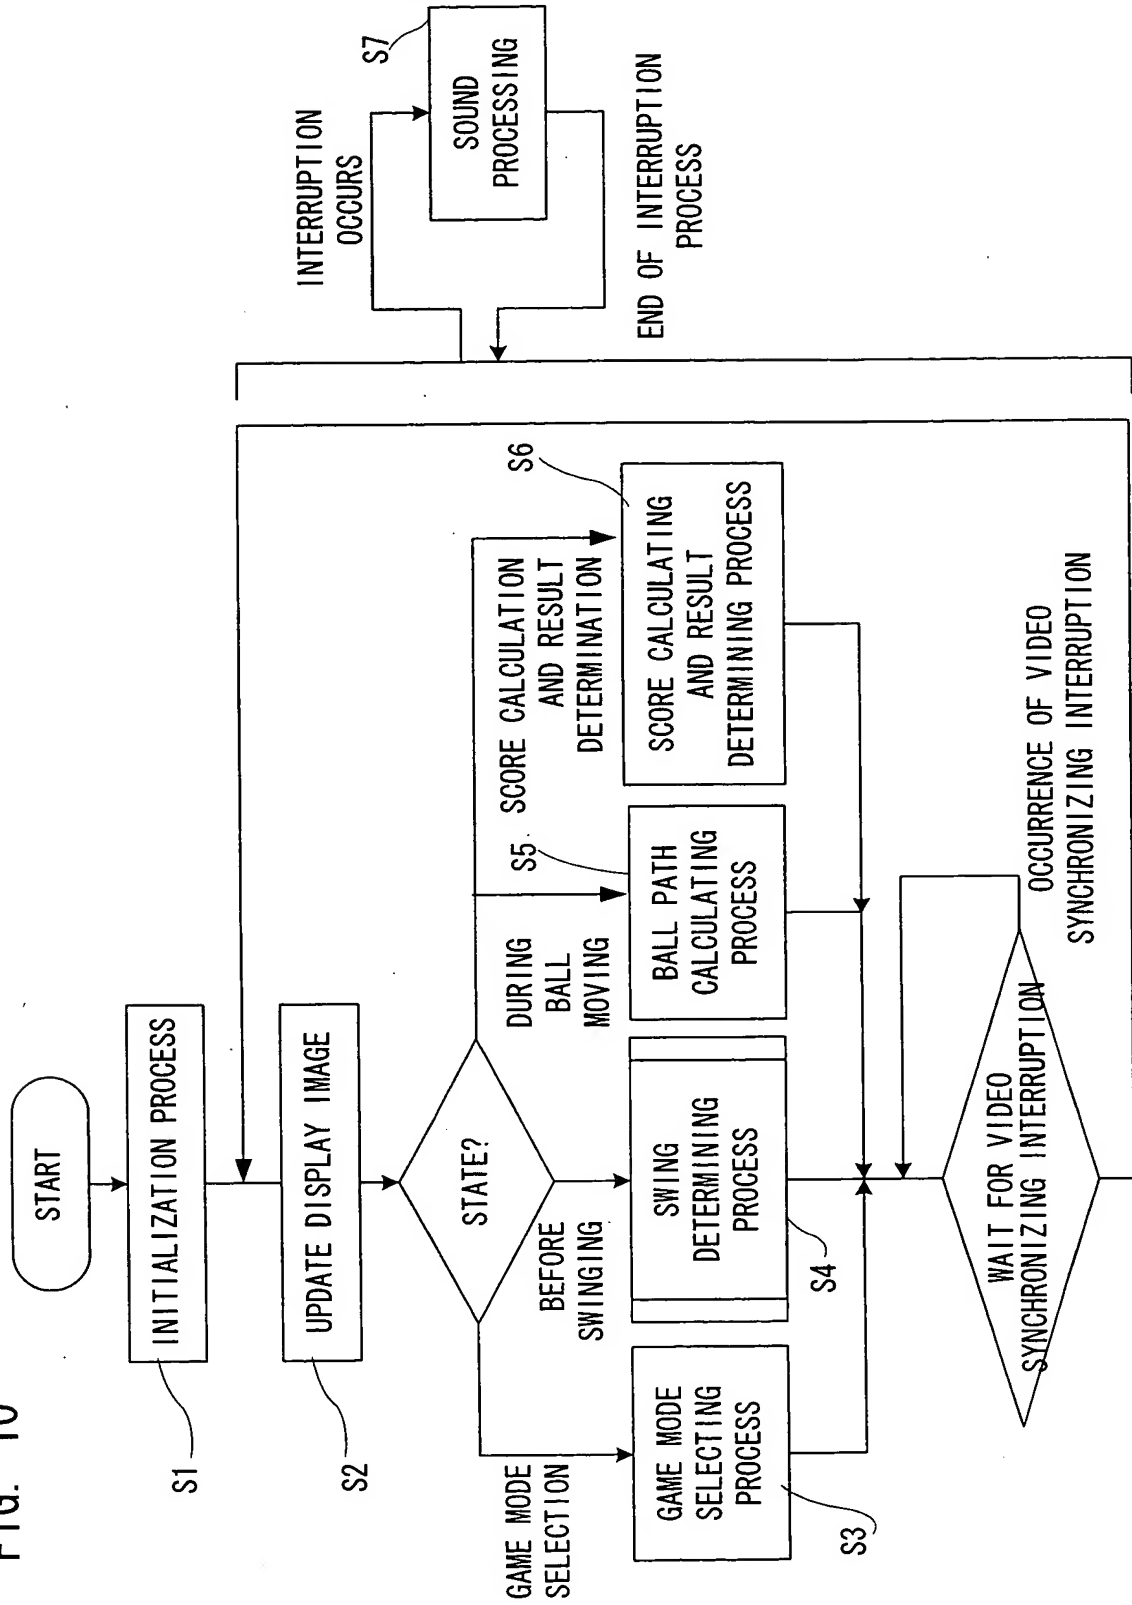


FIG. 11

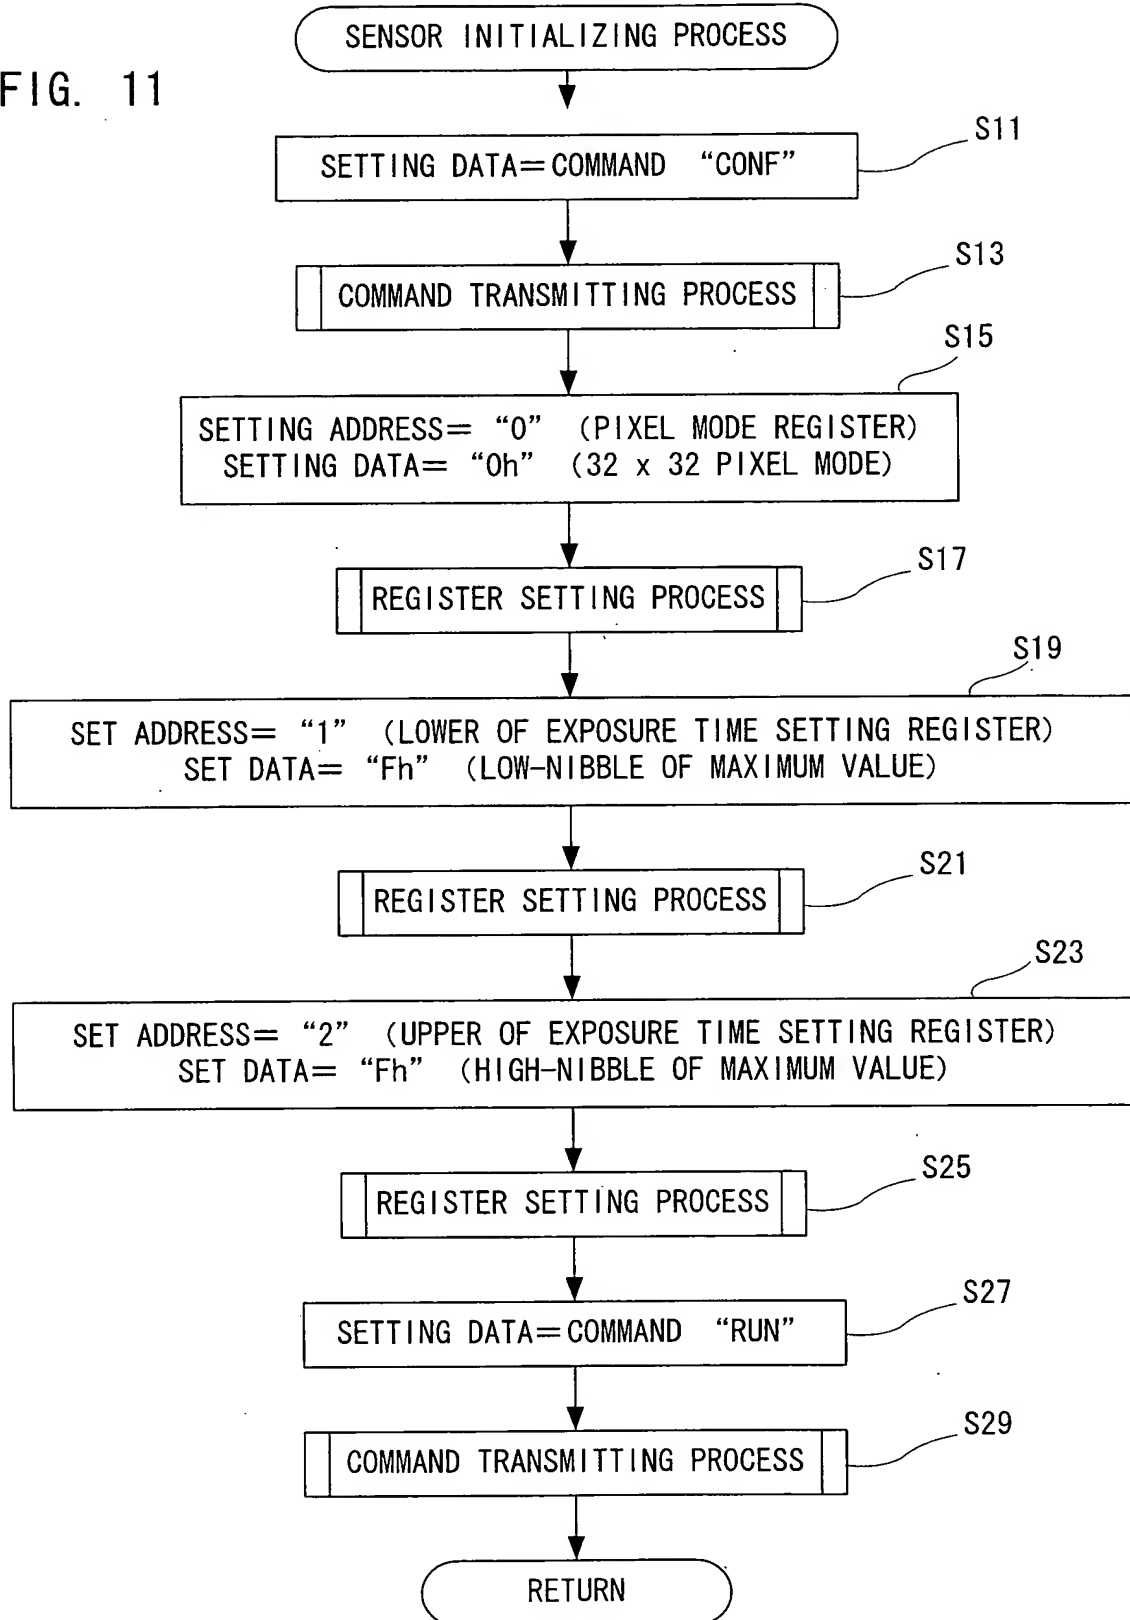


FIG. 12

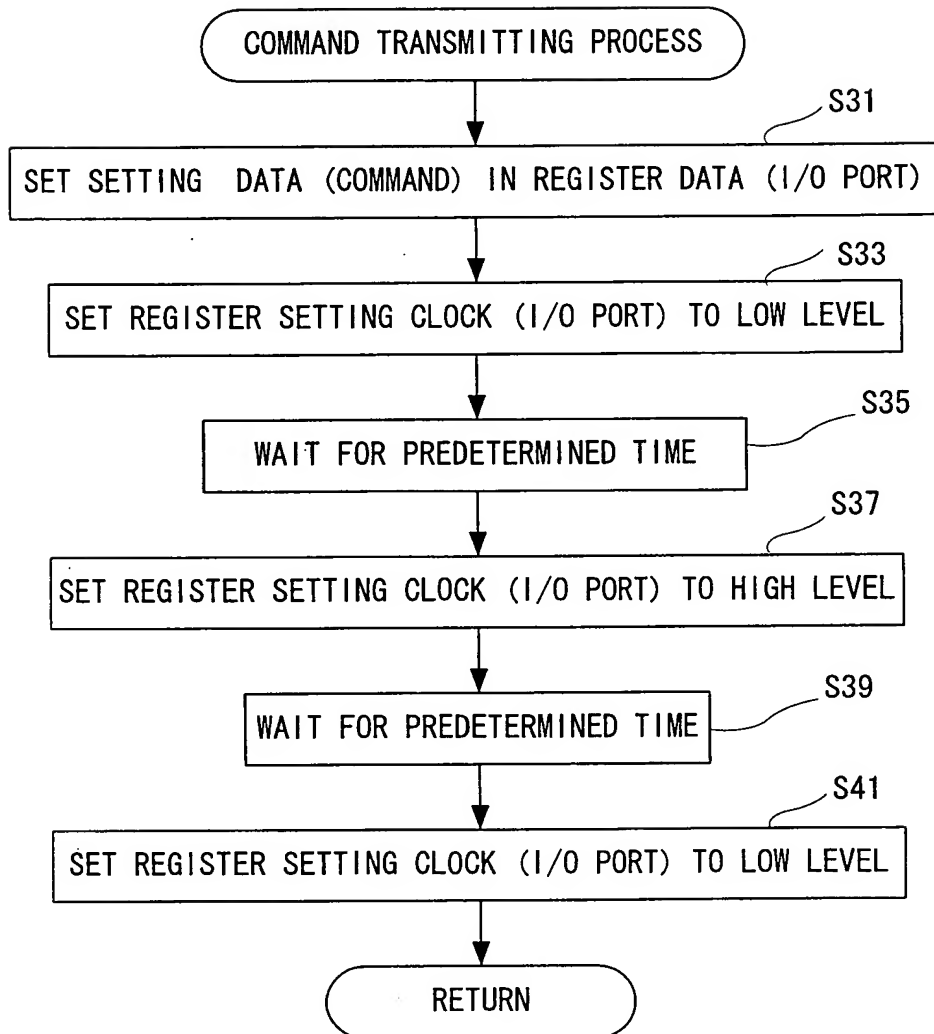


FIG. 13

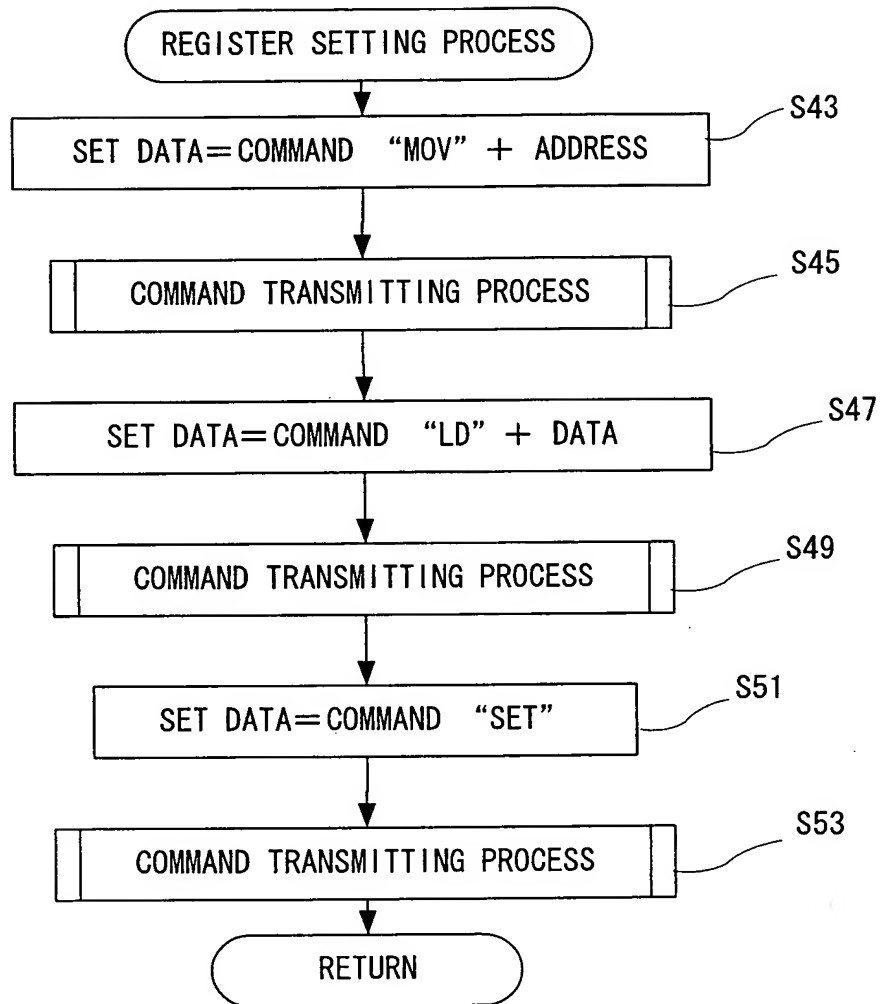


FIG. 14

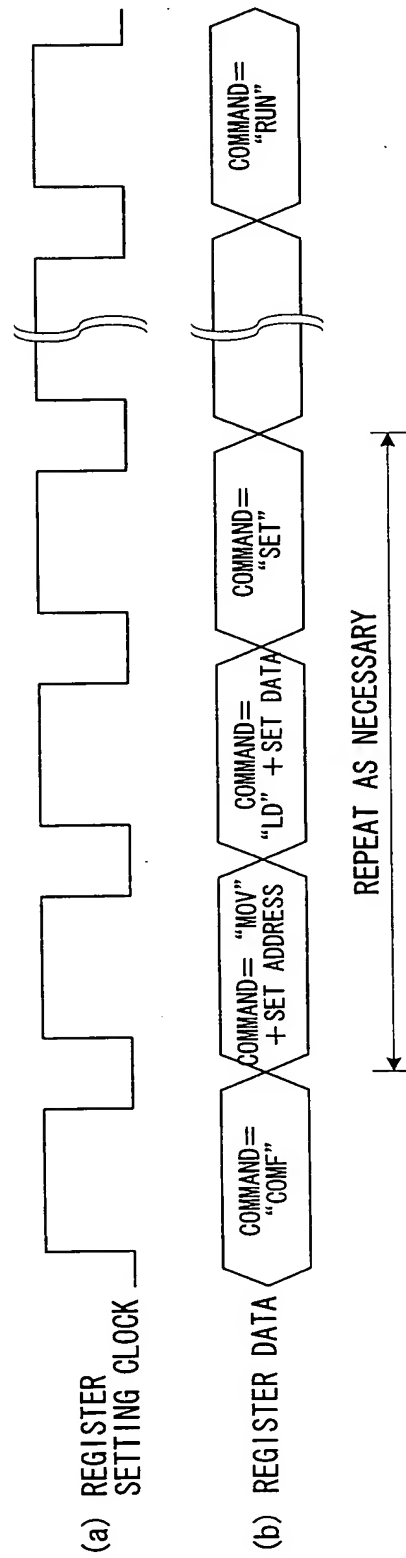


FIG. 15

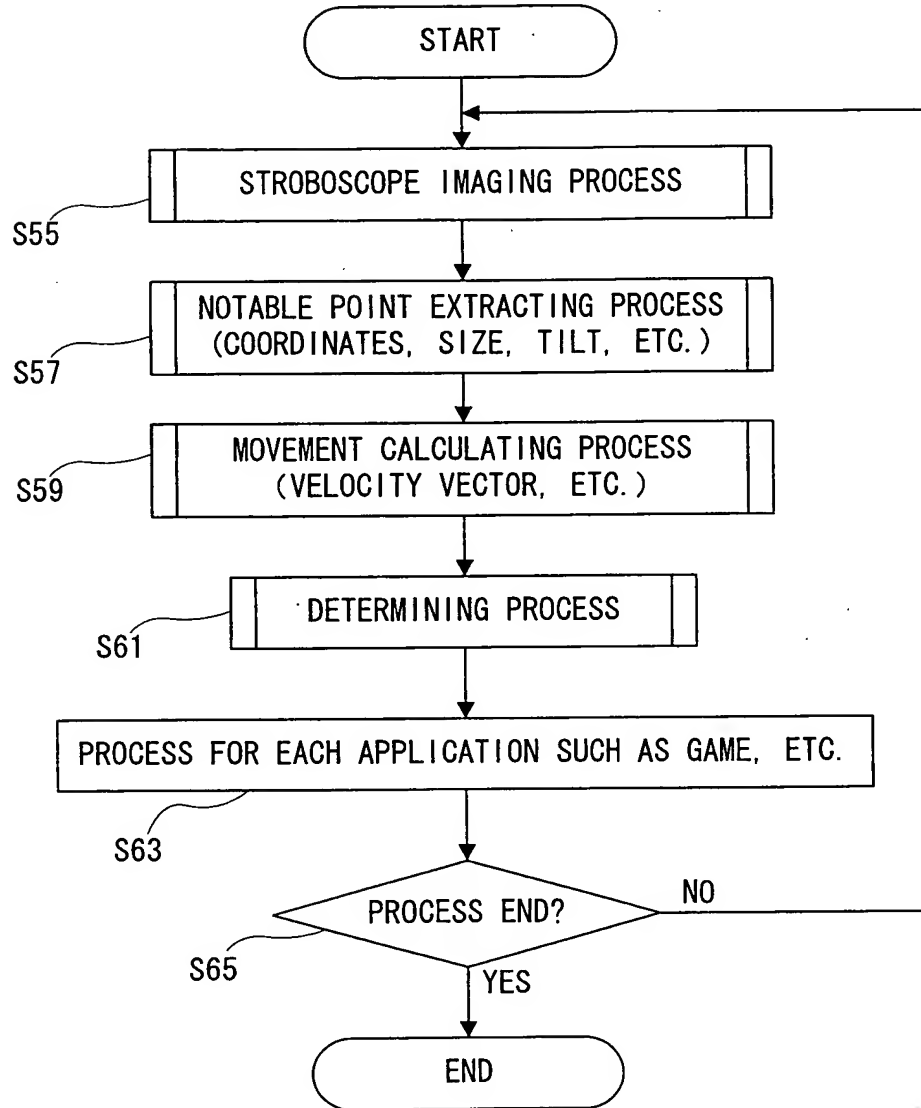


FIG. 16

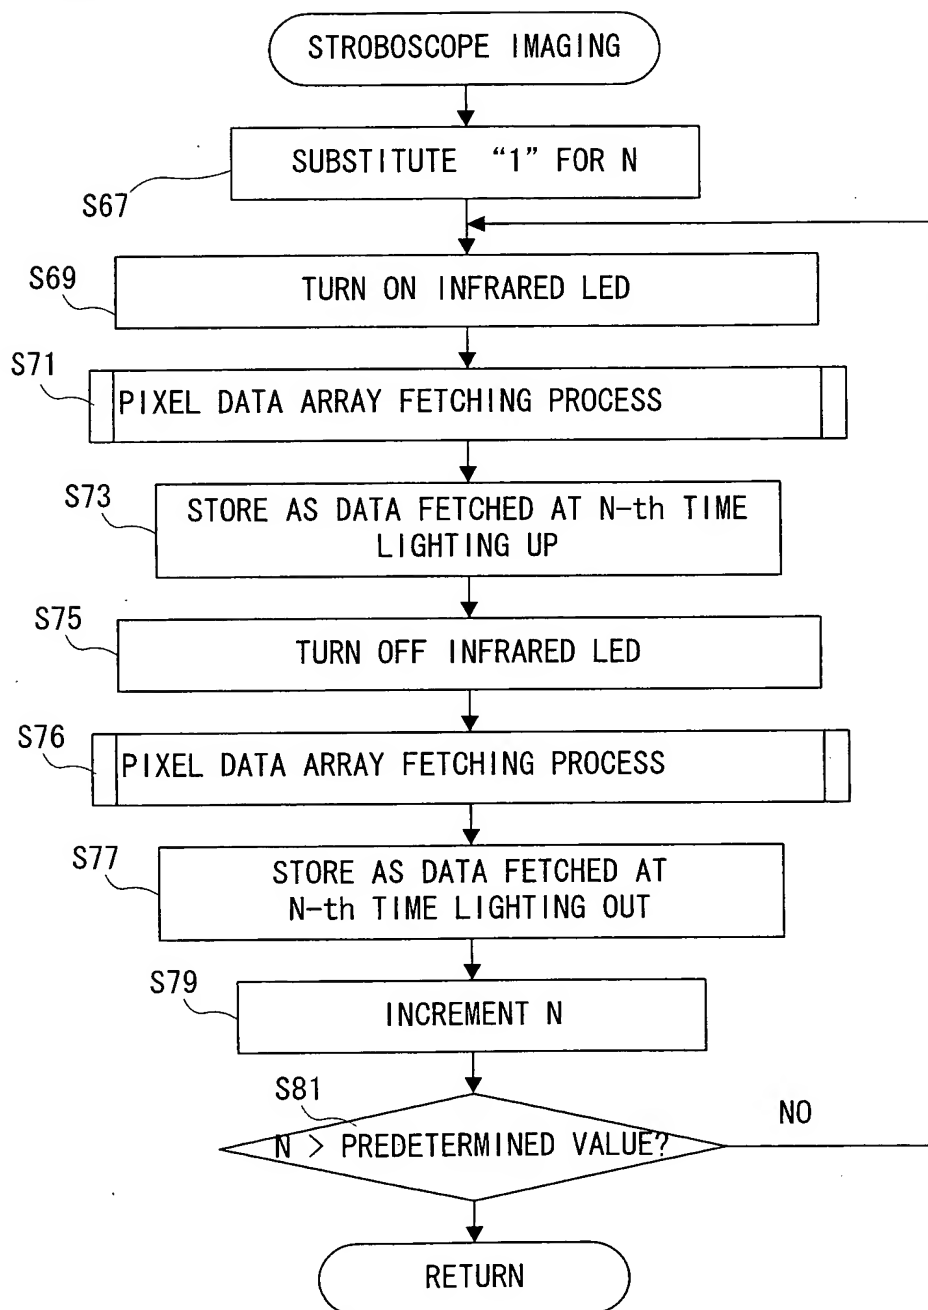


FIG. 17

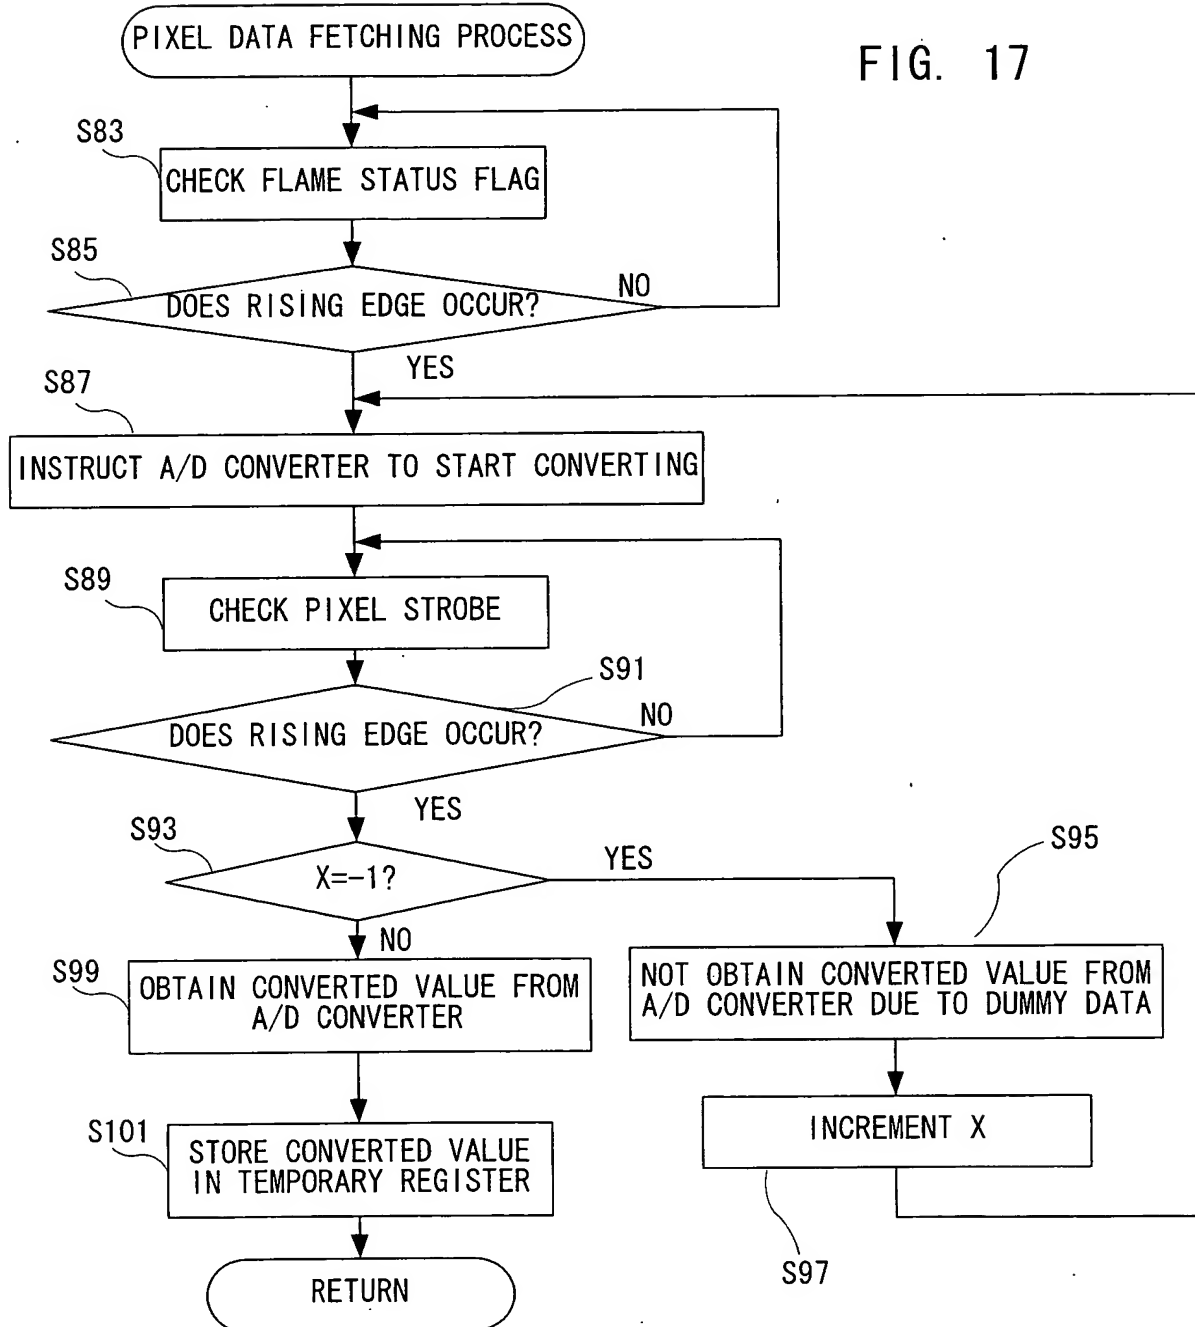


FIG. 18

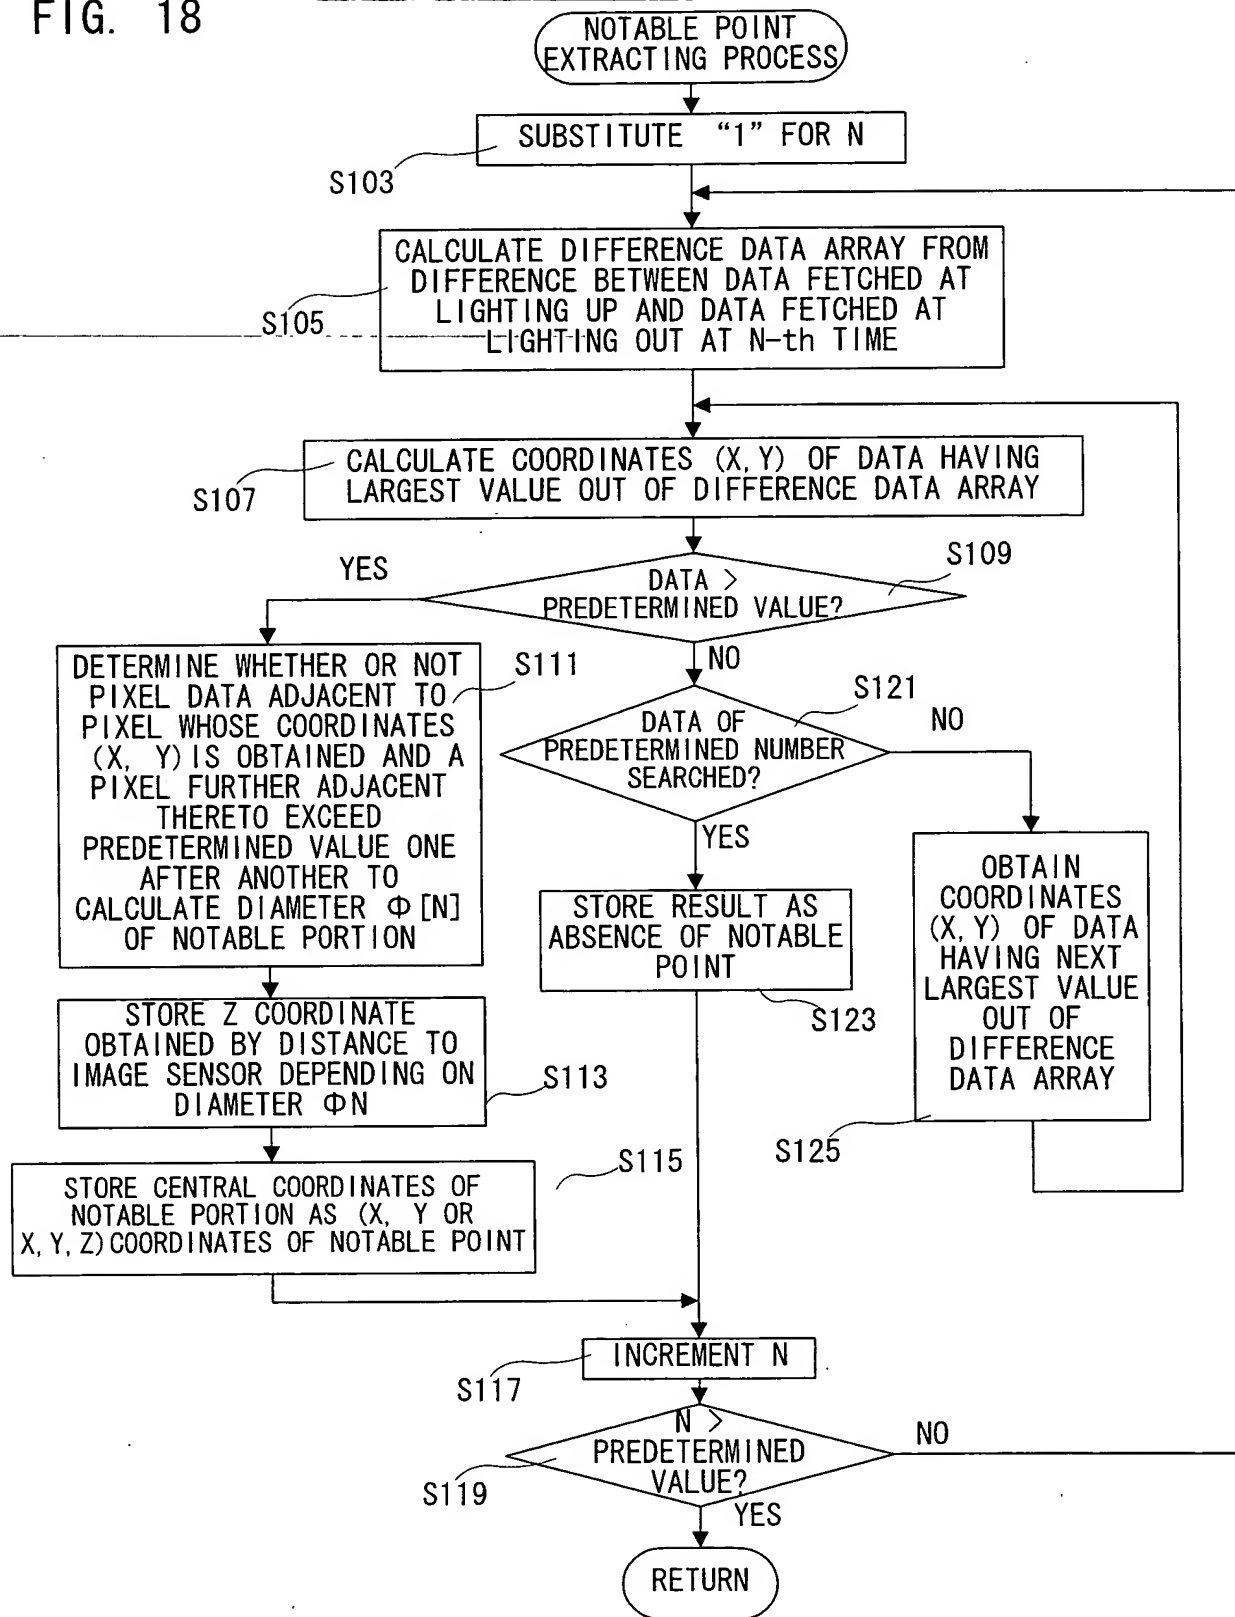


FIG. 19

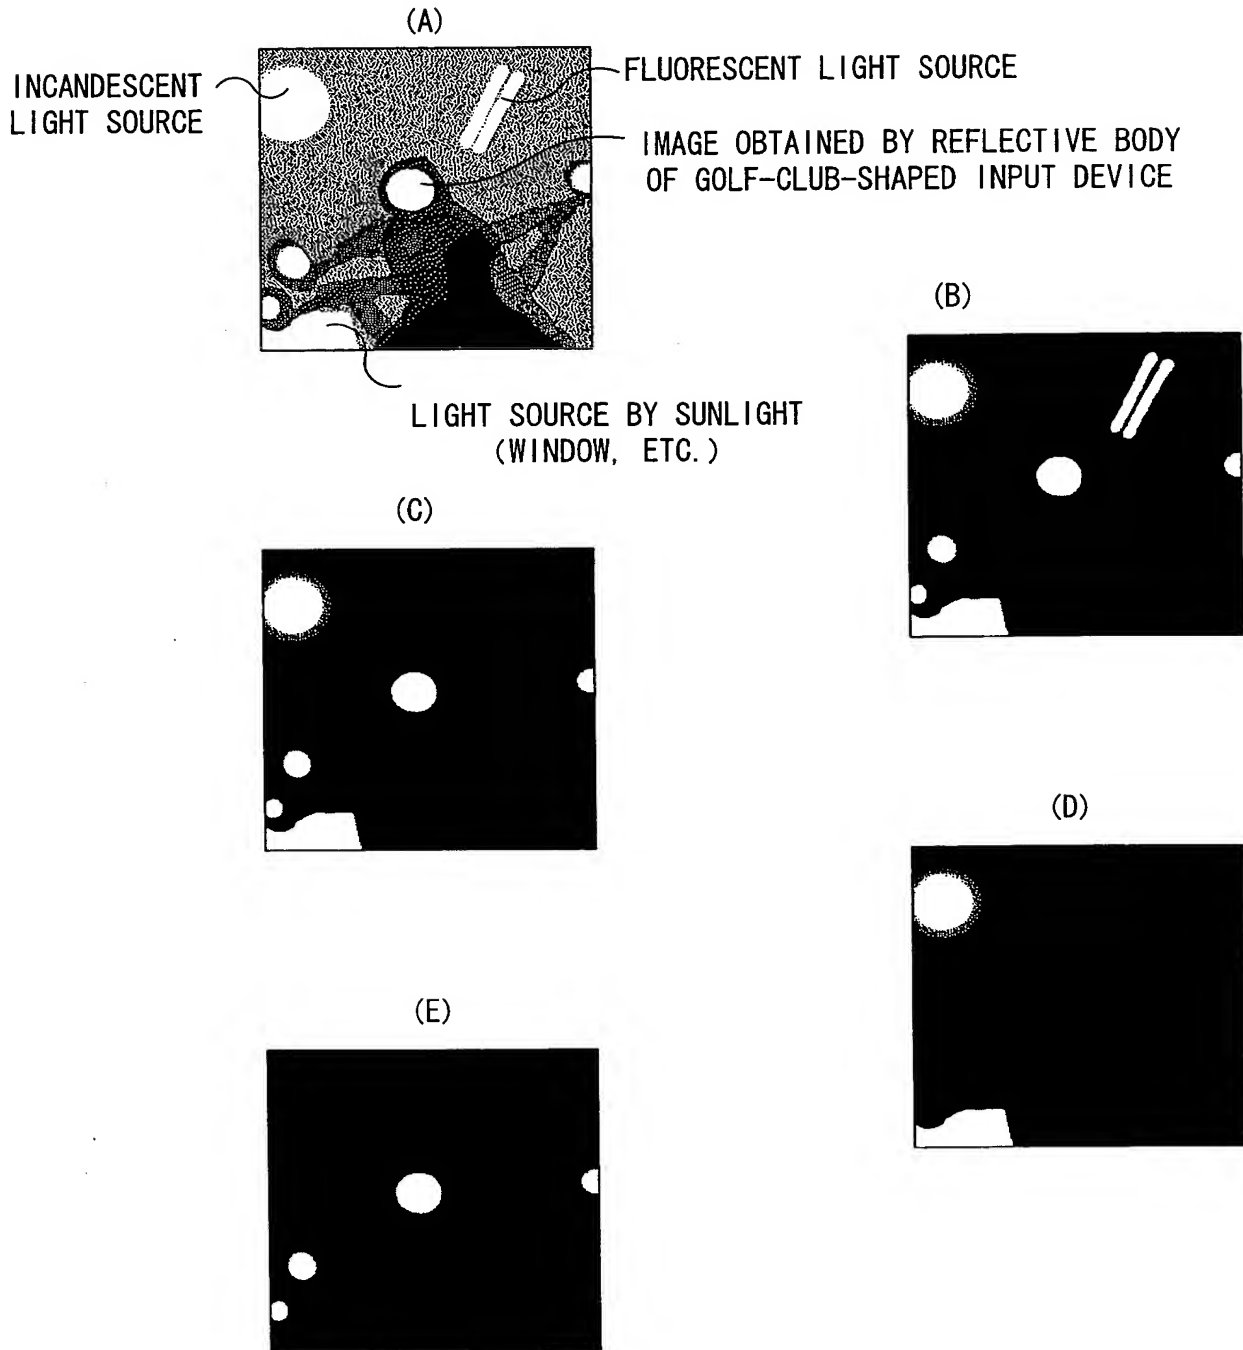


FIG. 20

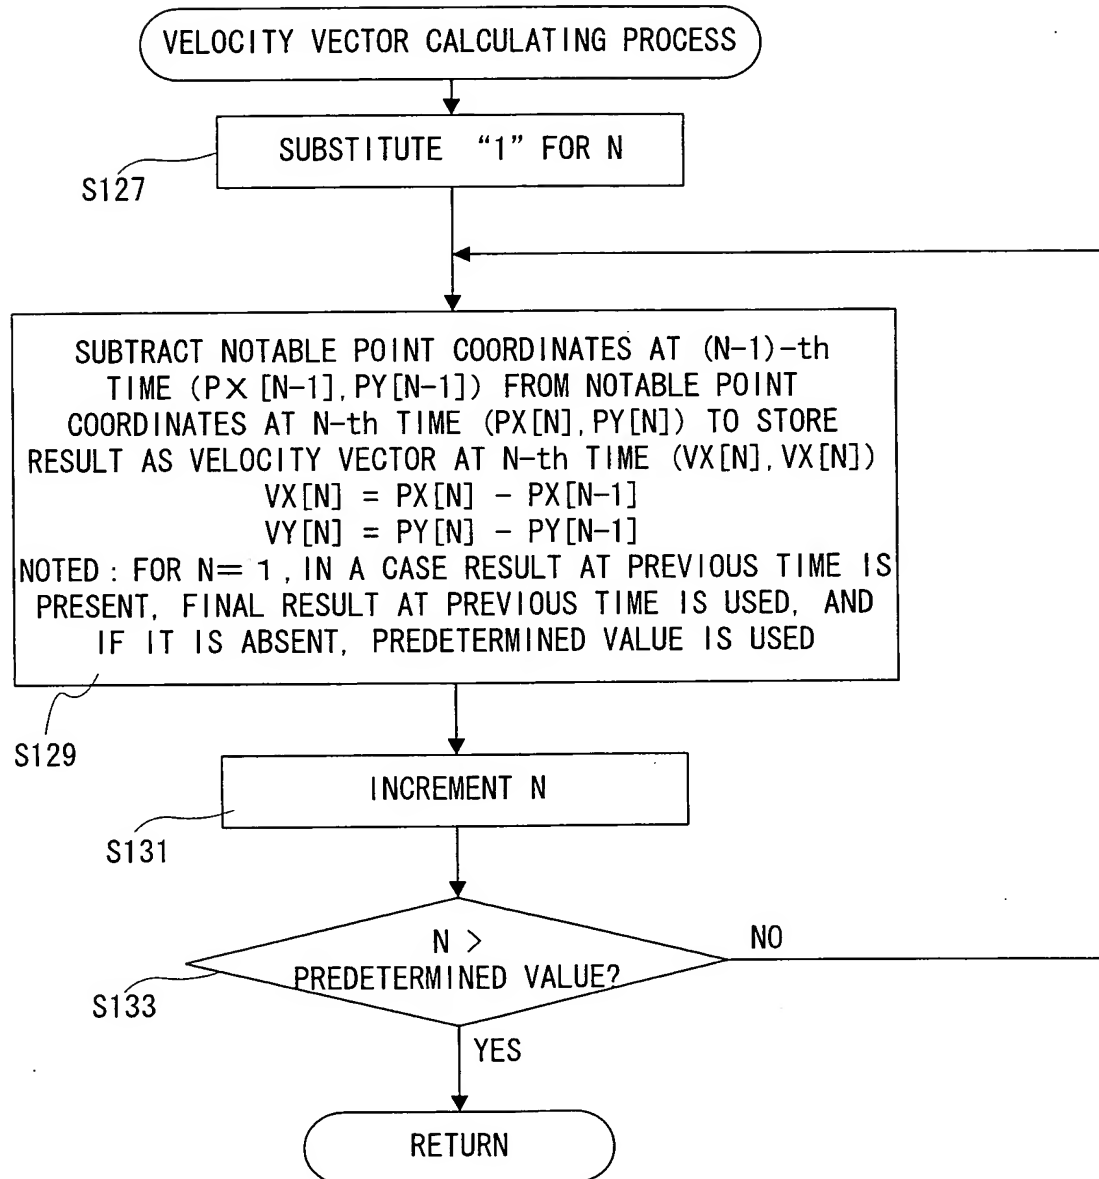


FIG. 21

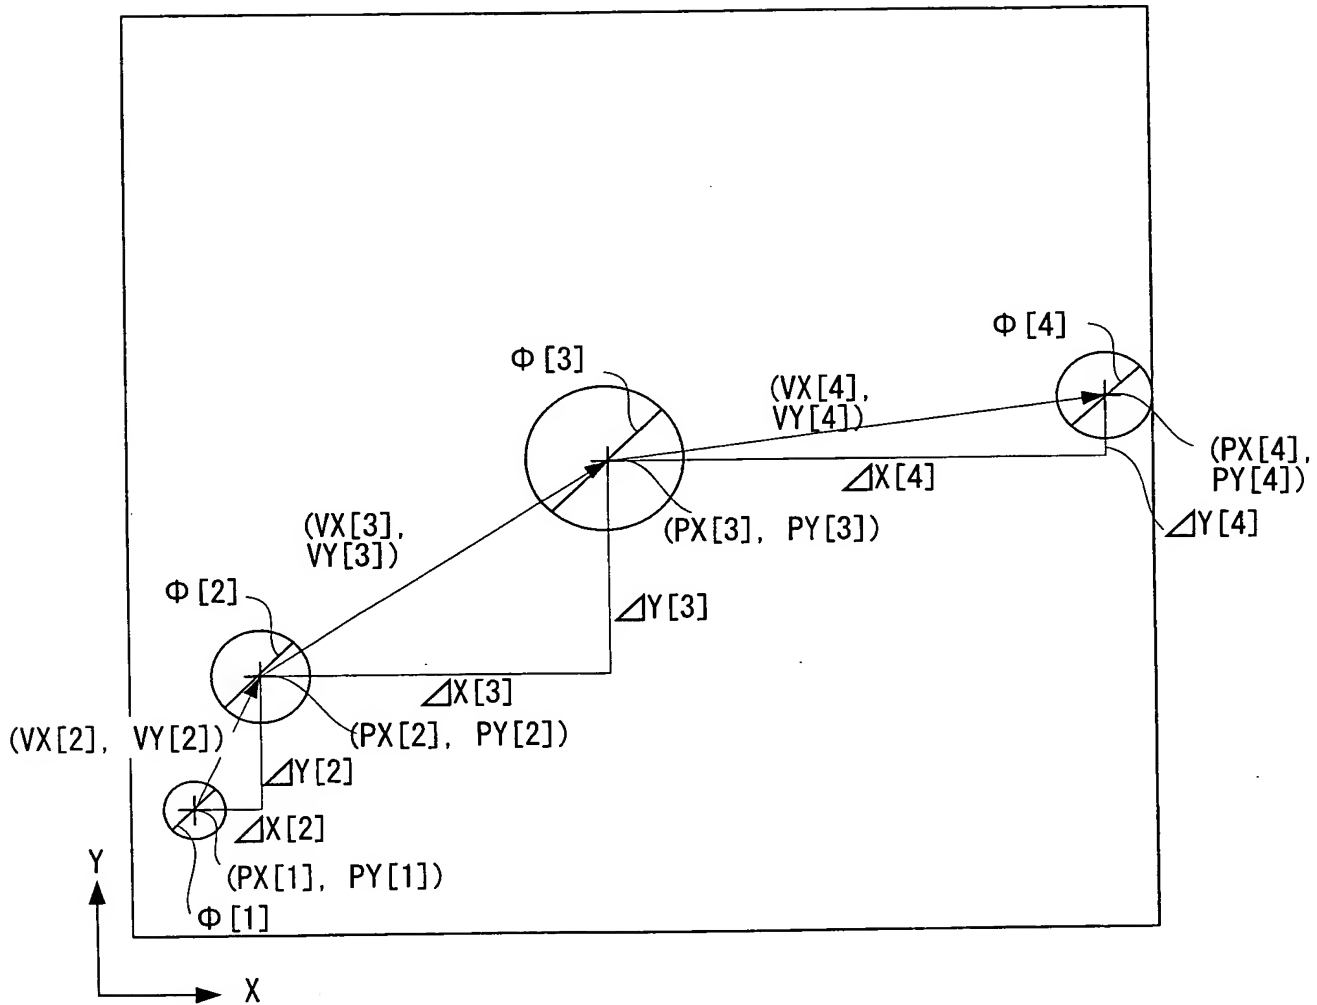


FIG. 22

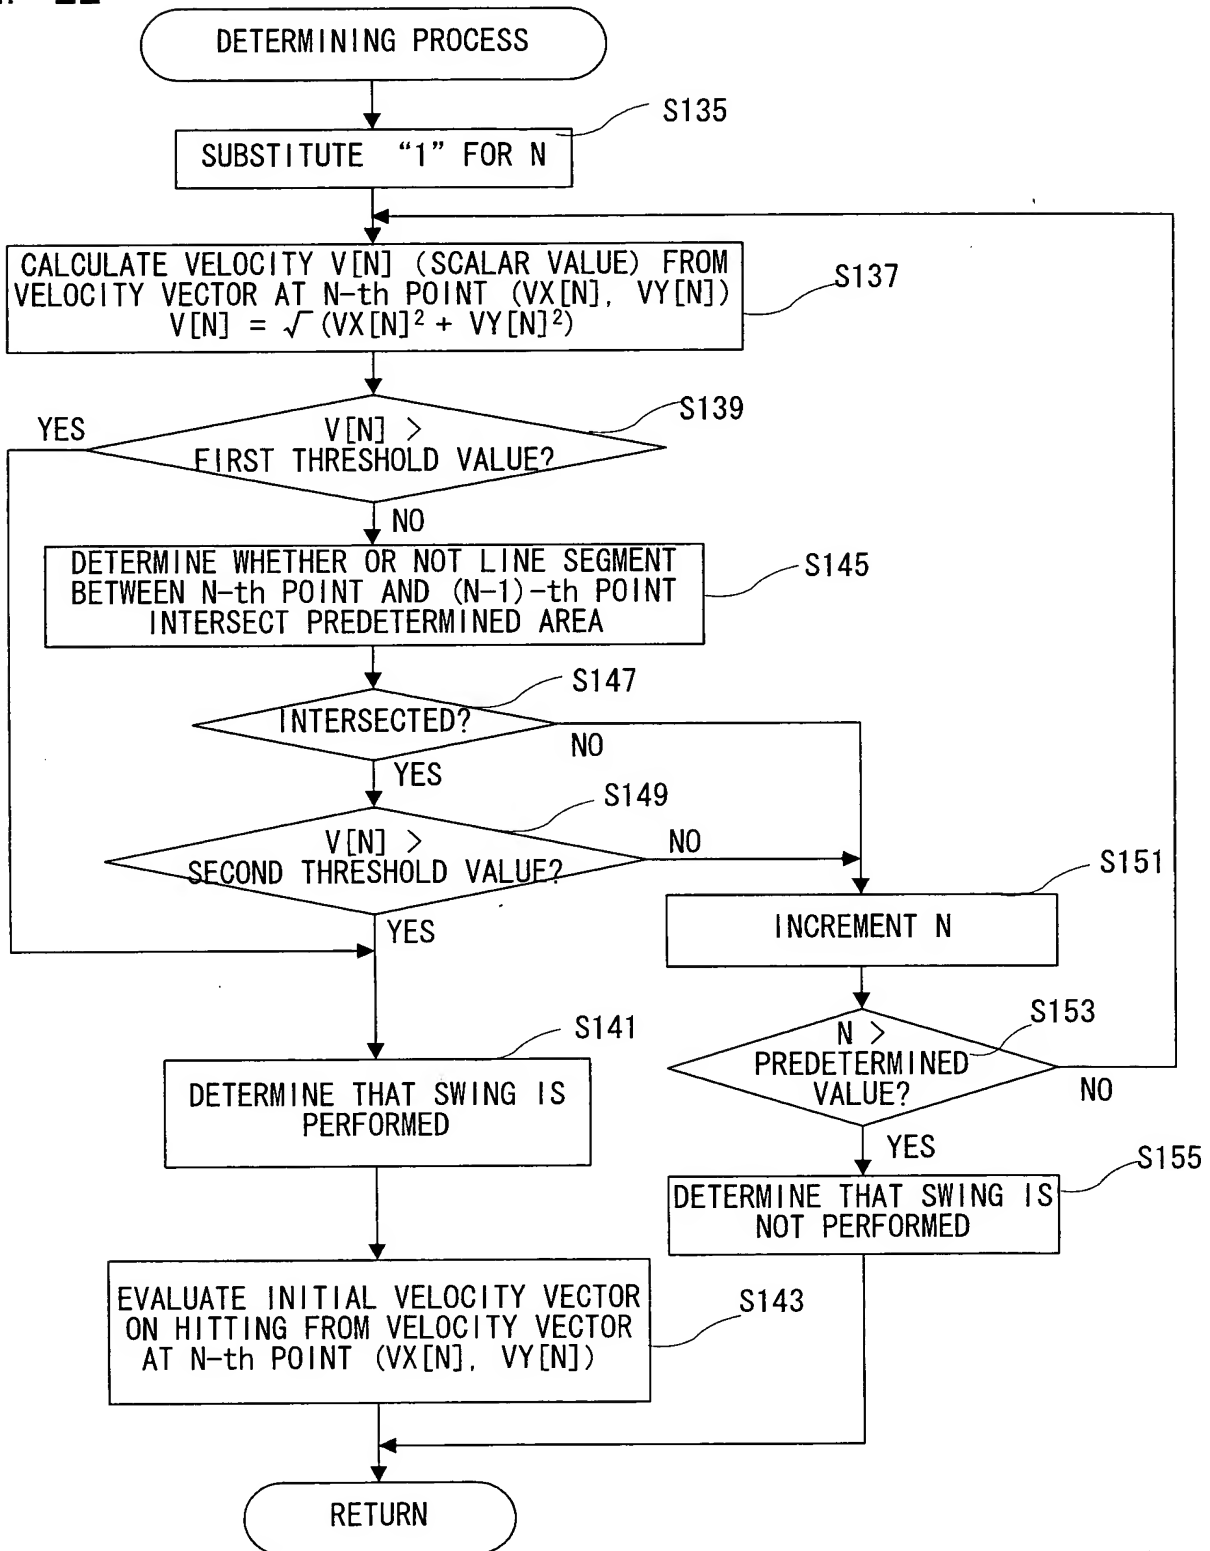


FIG. 23

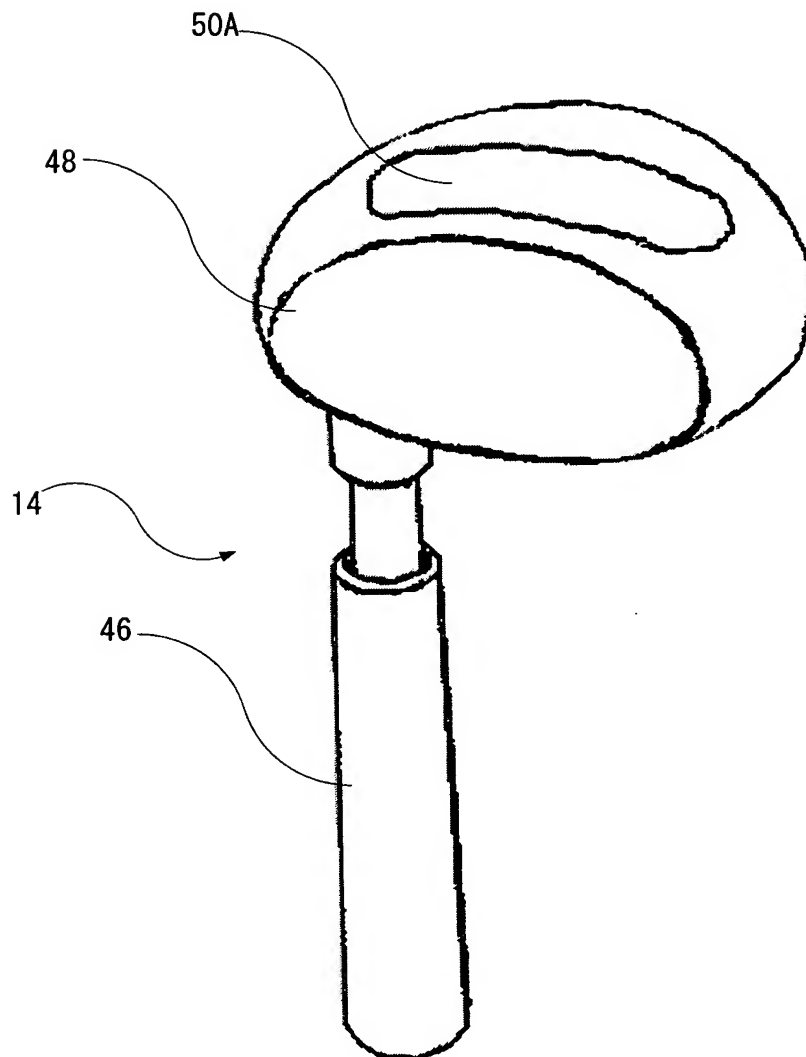


FIG. 24

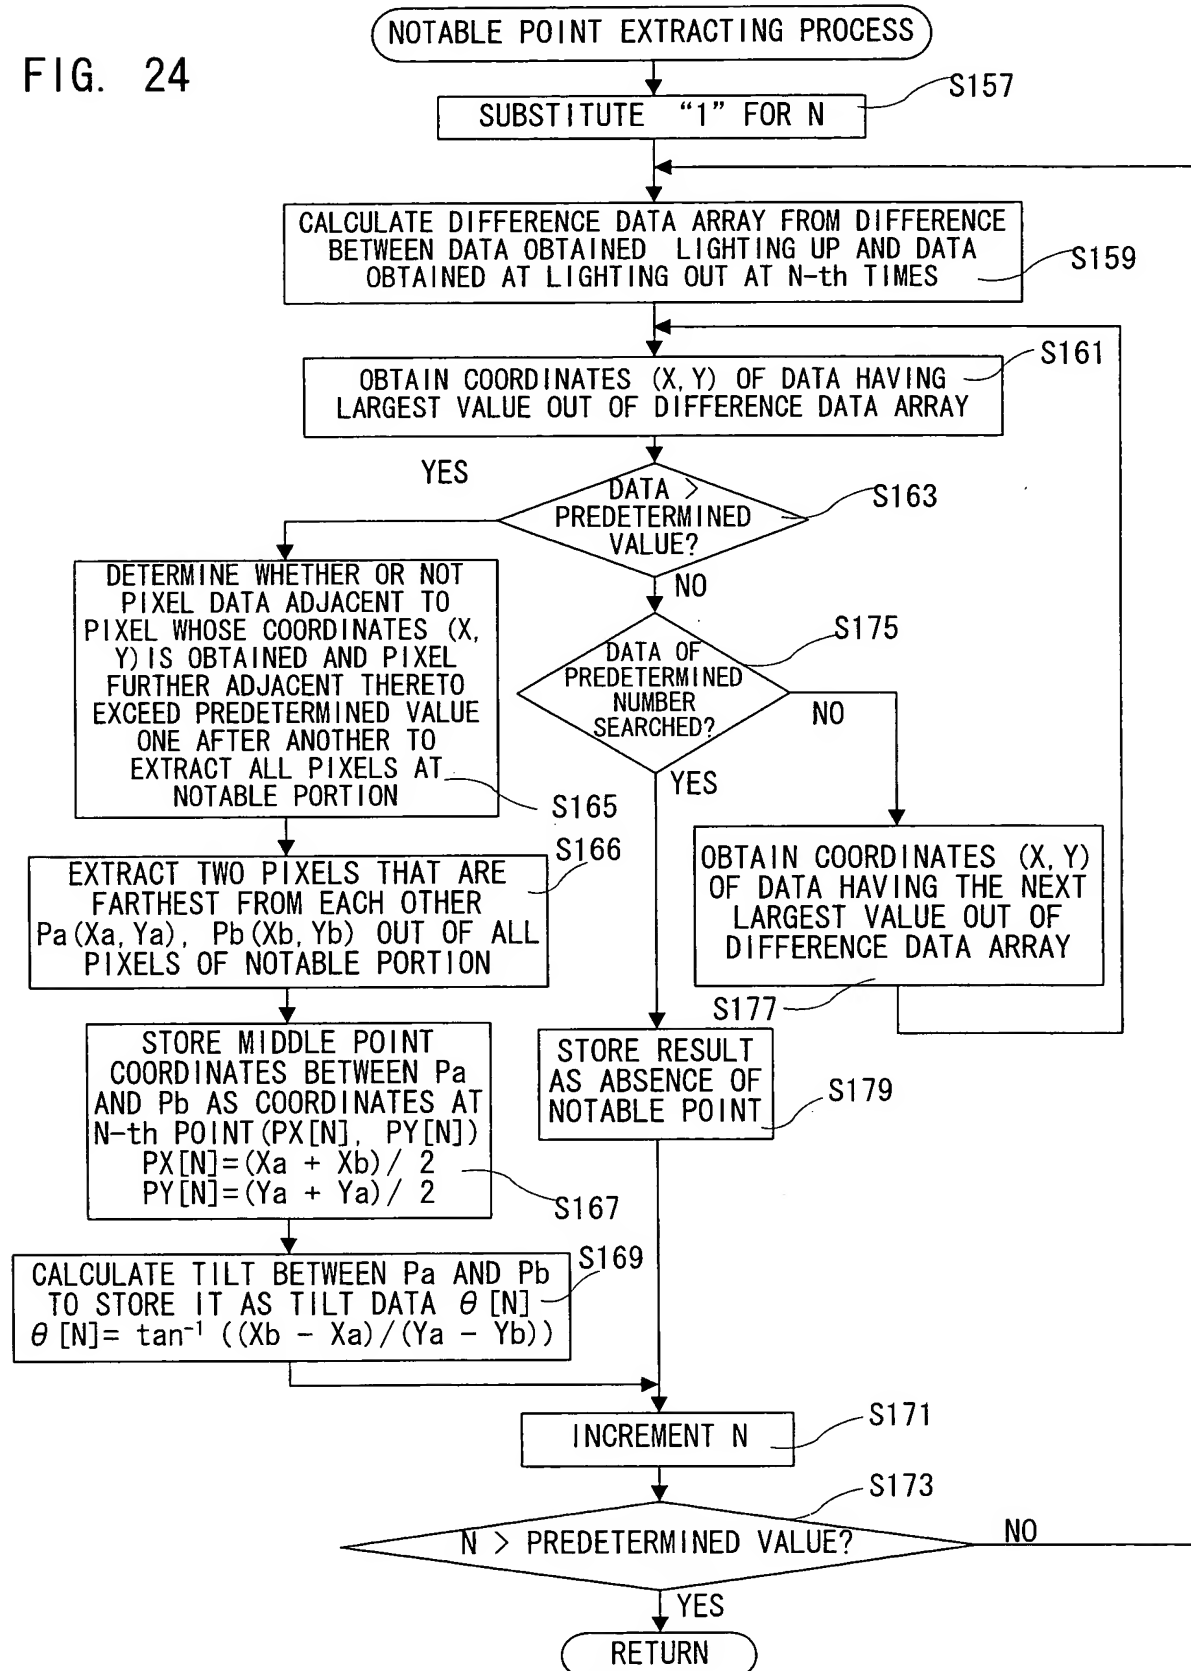


FIG. 25

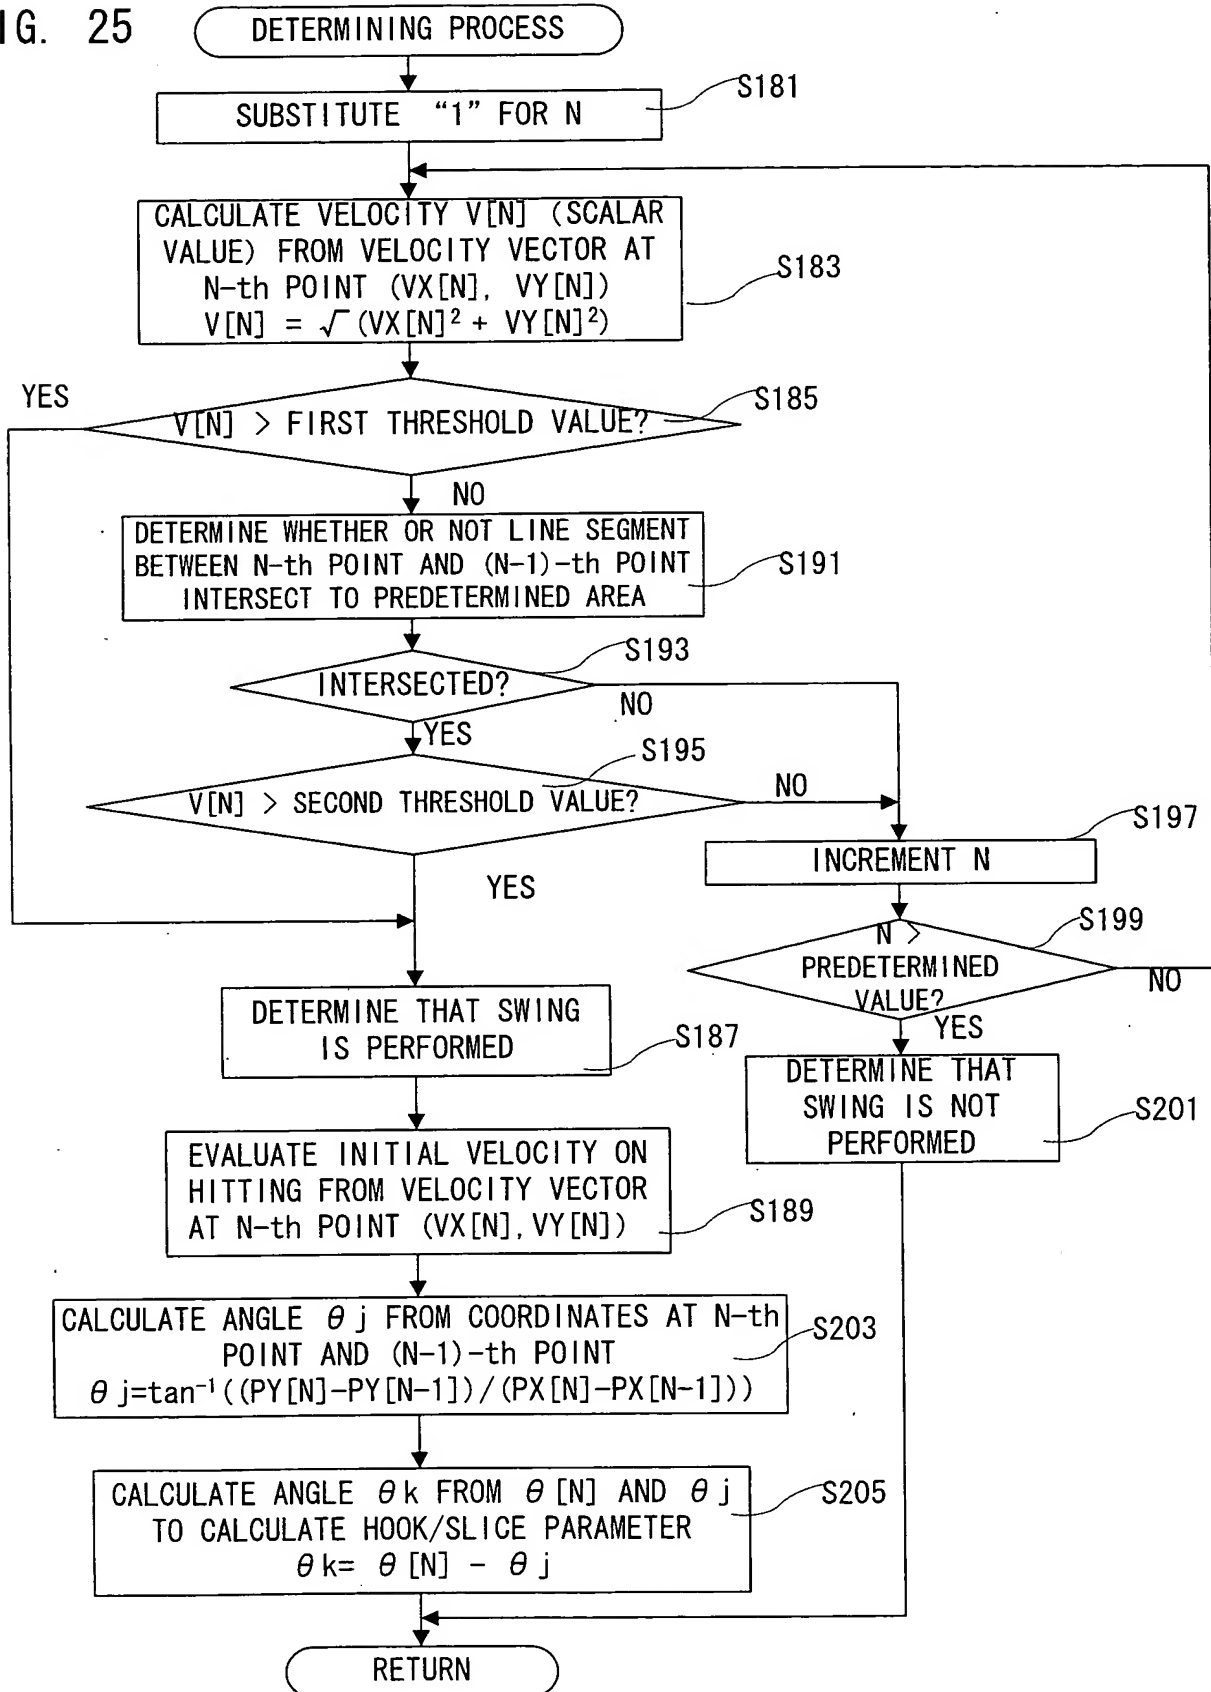


FIG. 26

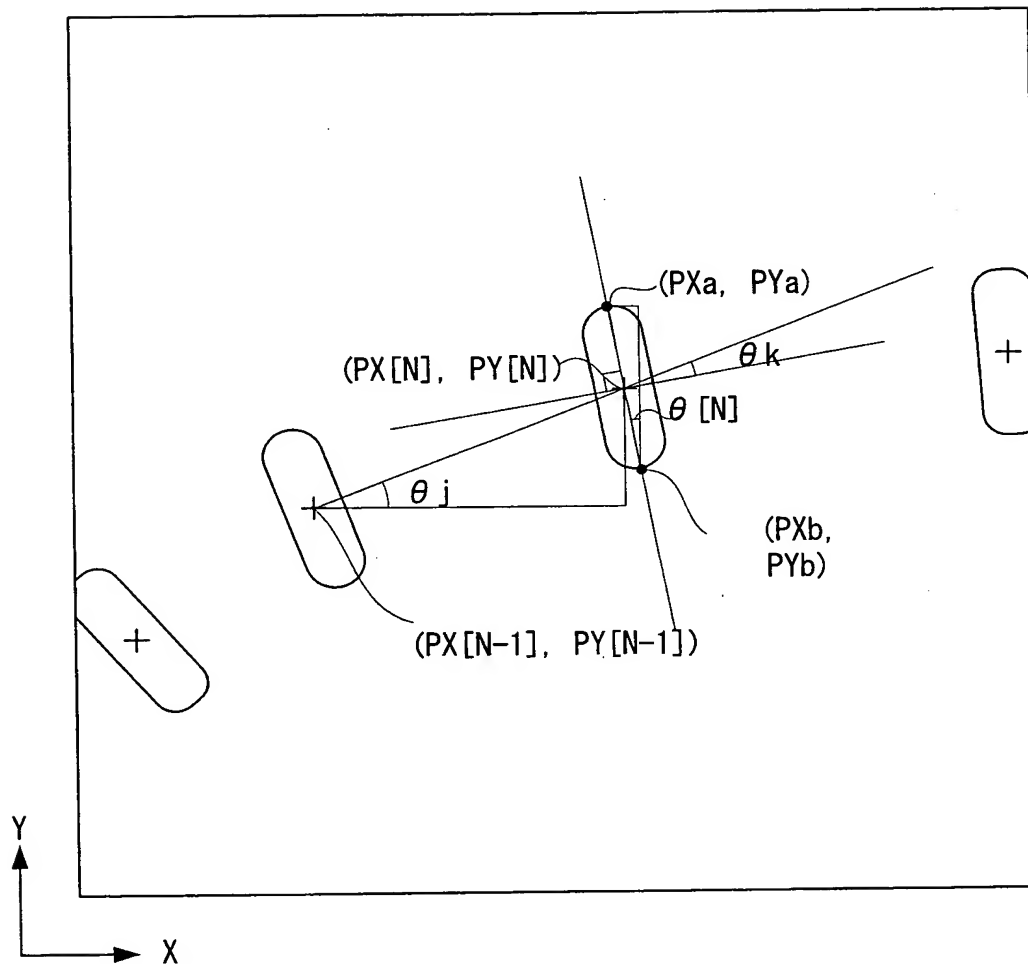


FIG. 1 is a schematic diagram of a medical device 16. The device includes a main body 78 with a handle 96 and a head 80. The head 80 features a display 82, a control panel 40 with buttons 42, and a sensor array 84. A cable 16 connects the device to a power source or data system. Cross-sectional views are indicated by arrows II X VII and II X VIII.

FIG. 28

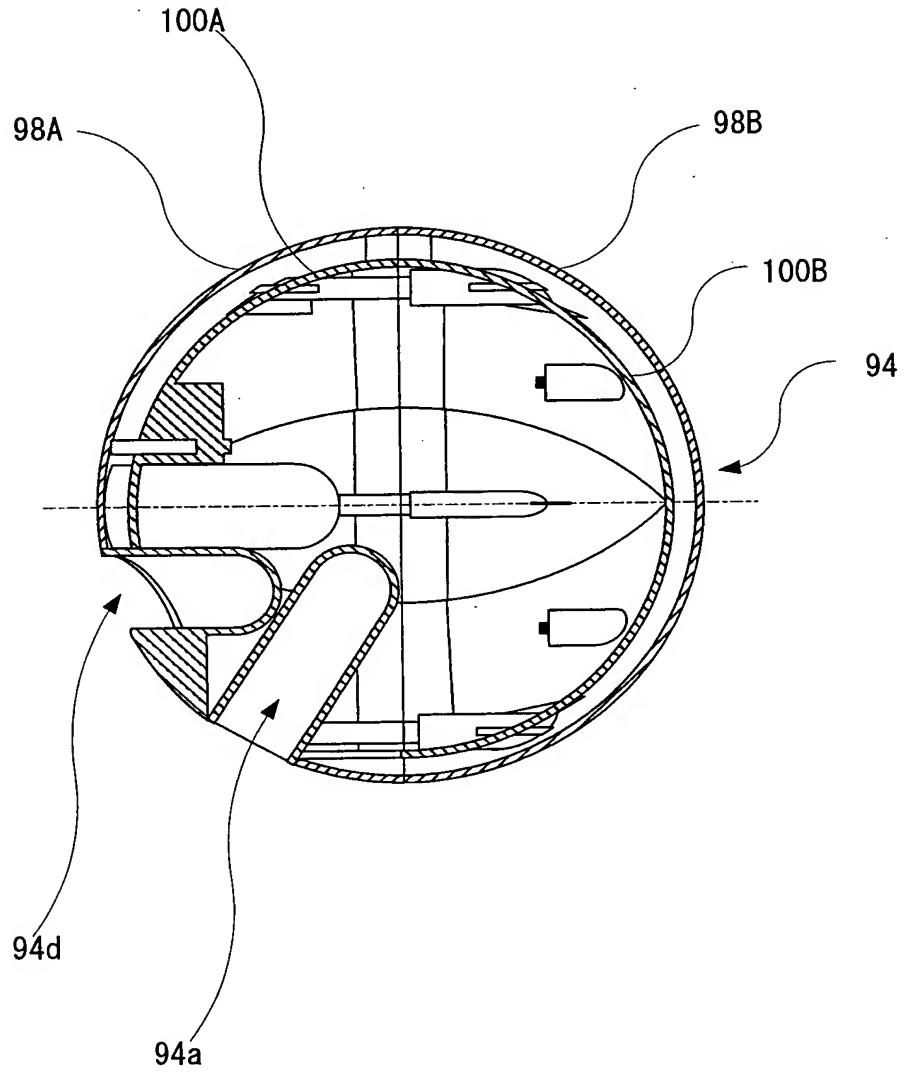


FIG. 29

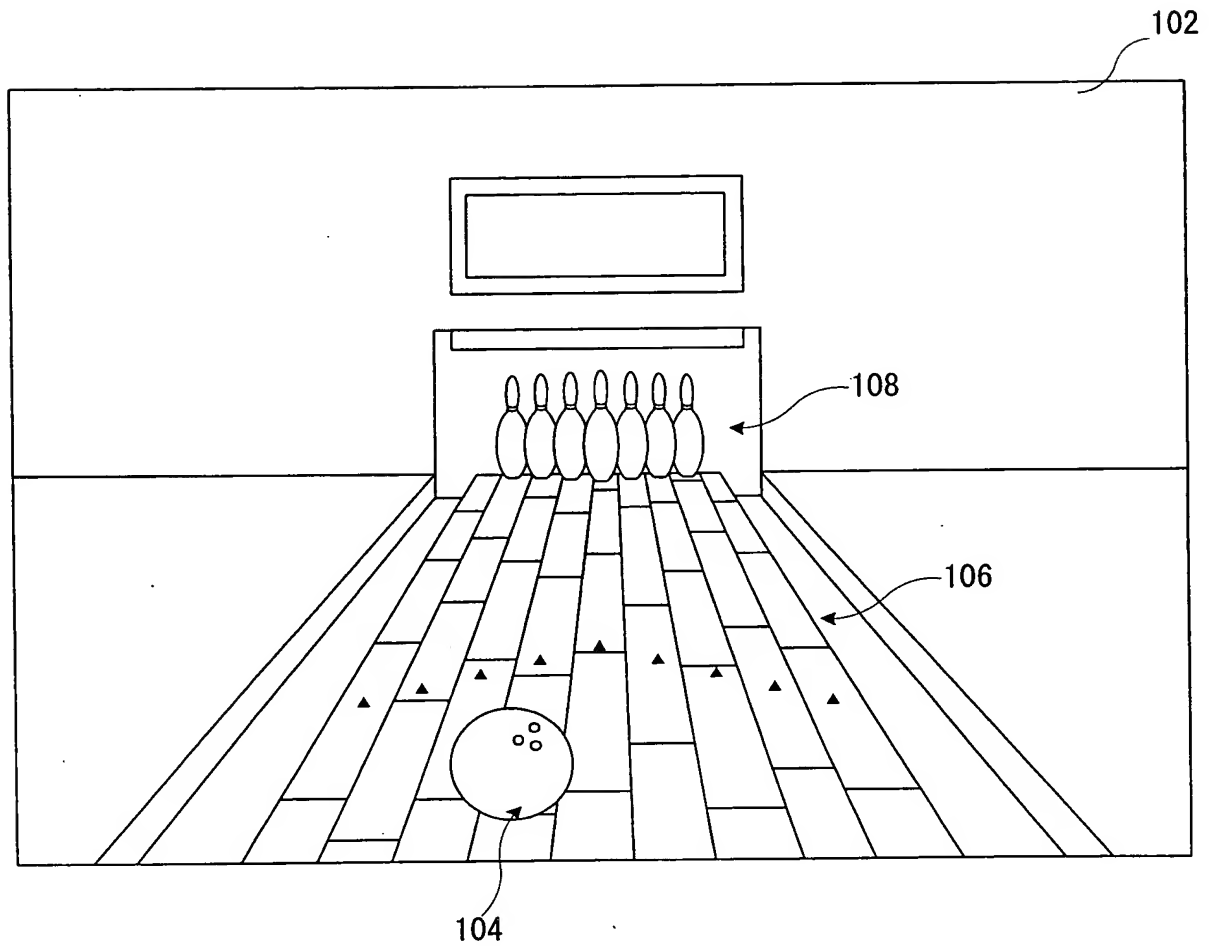


FIG. 30

SCORE SHEET

110

	1	2	3	4	5	6	7	8	9	10
A B C	G -	1 2	3 4							
	0	3	10							
	1	2	3	4	5	6	7	8	9	10
D E F	6 1	5 2	3 3							
	8	15	21							
	1	2	3	4	5	6	7	8	9	10
G H I	1 G	3 5	5 1							
	8	9	15							
	1	2	3	4	5	6	7	8	9	10
J K L	9 0	3 2	7 2							
	9	14	23							

FIG. 31

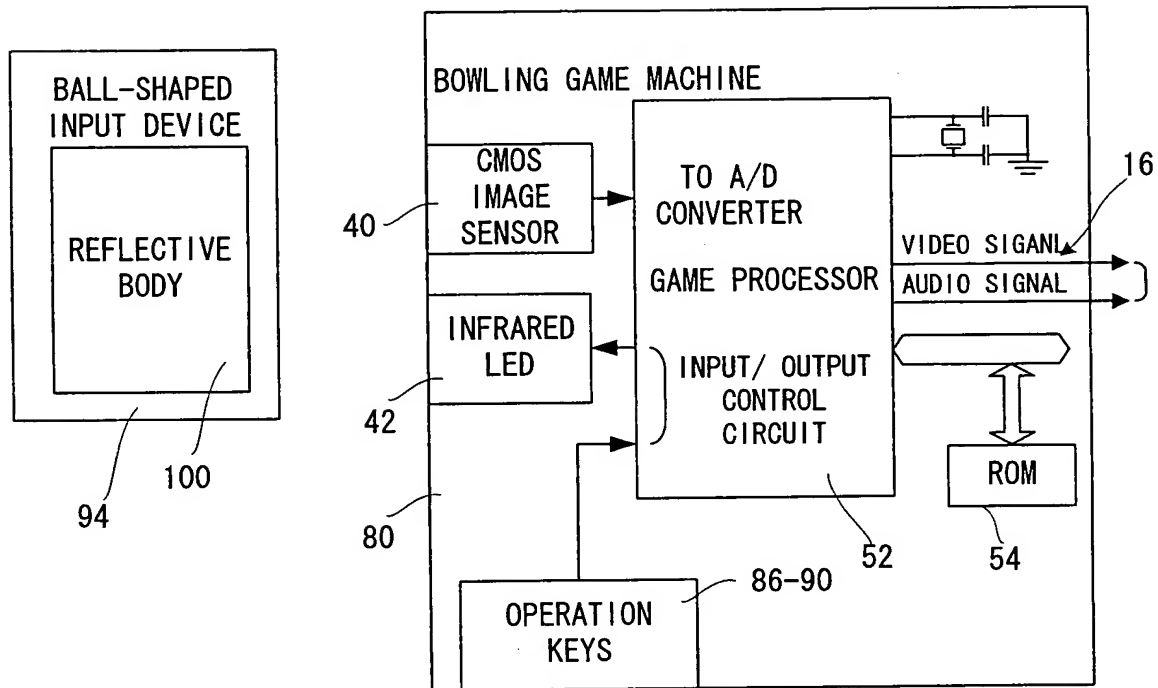


FIG. 32

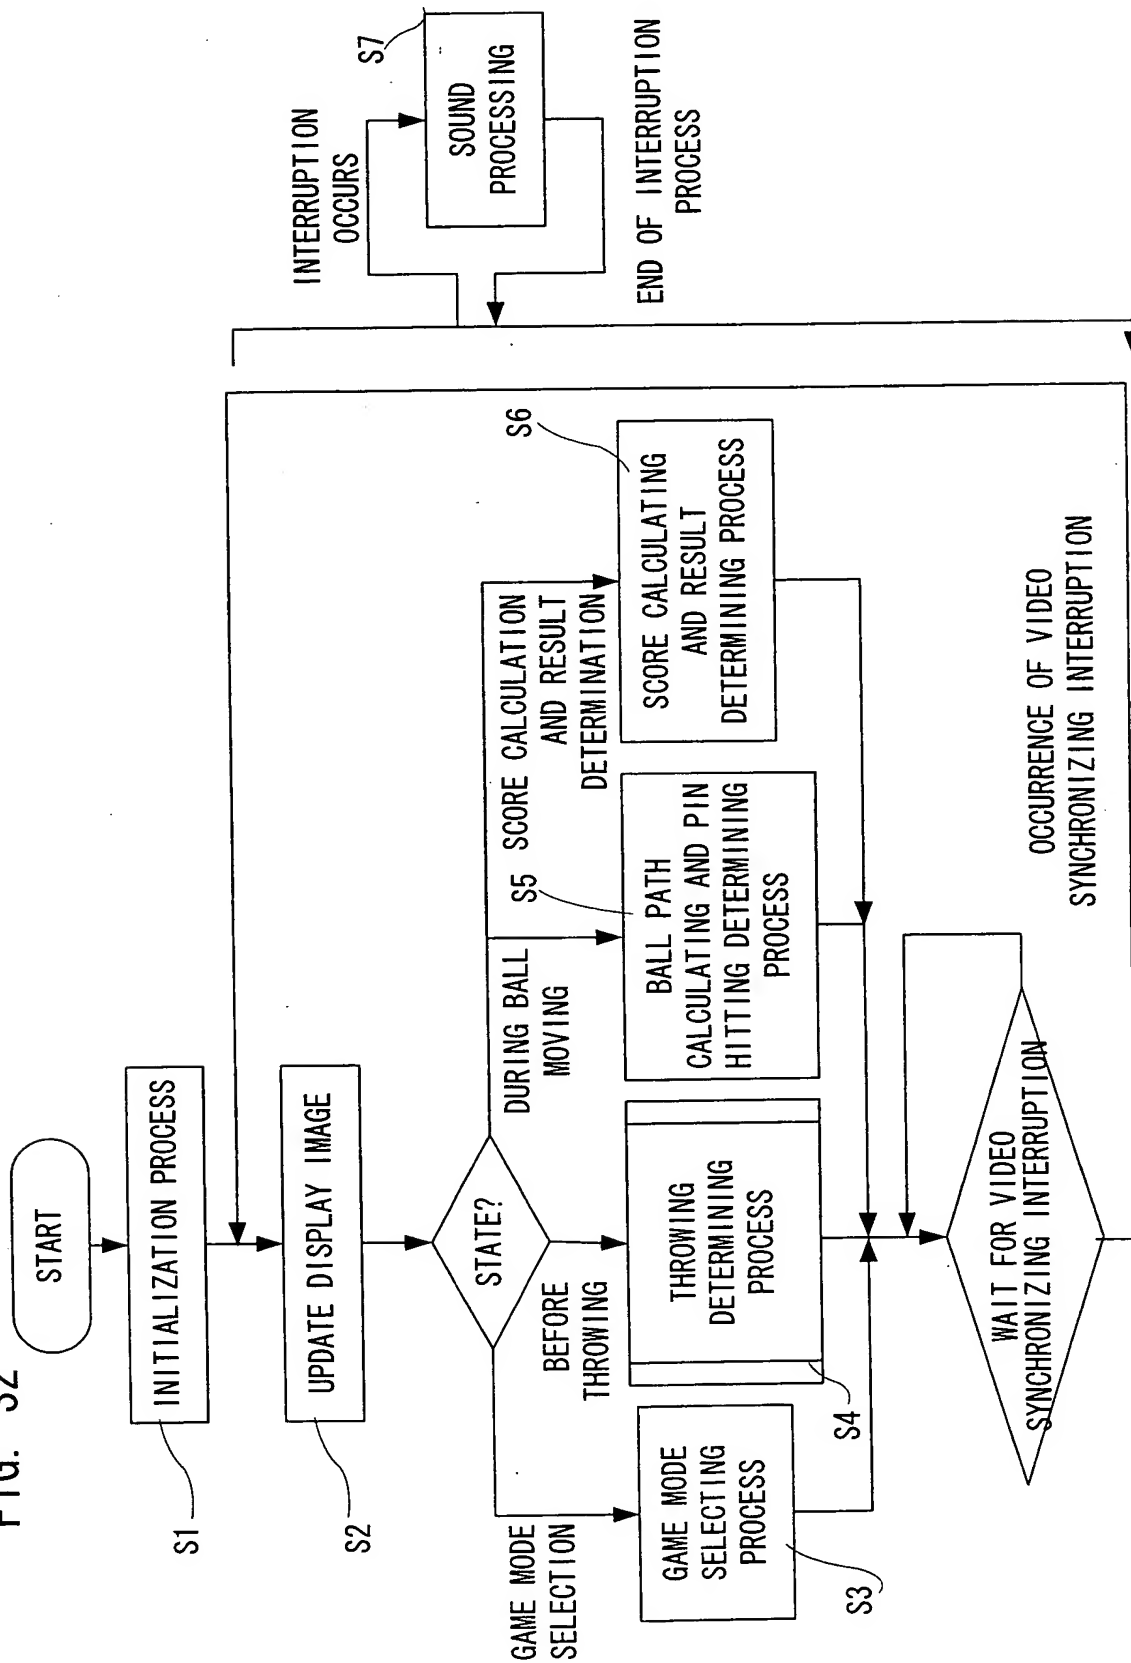


FIG. 33

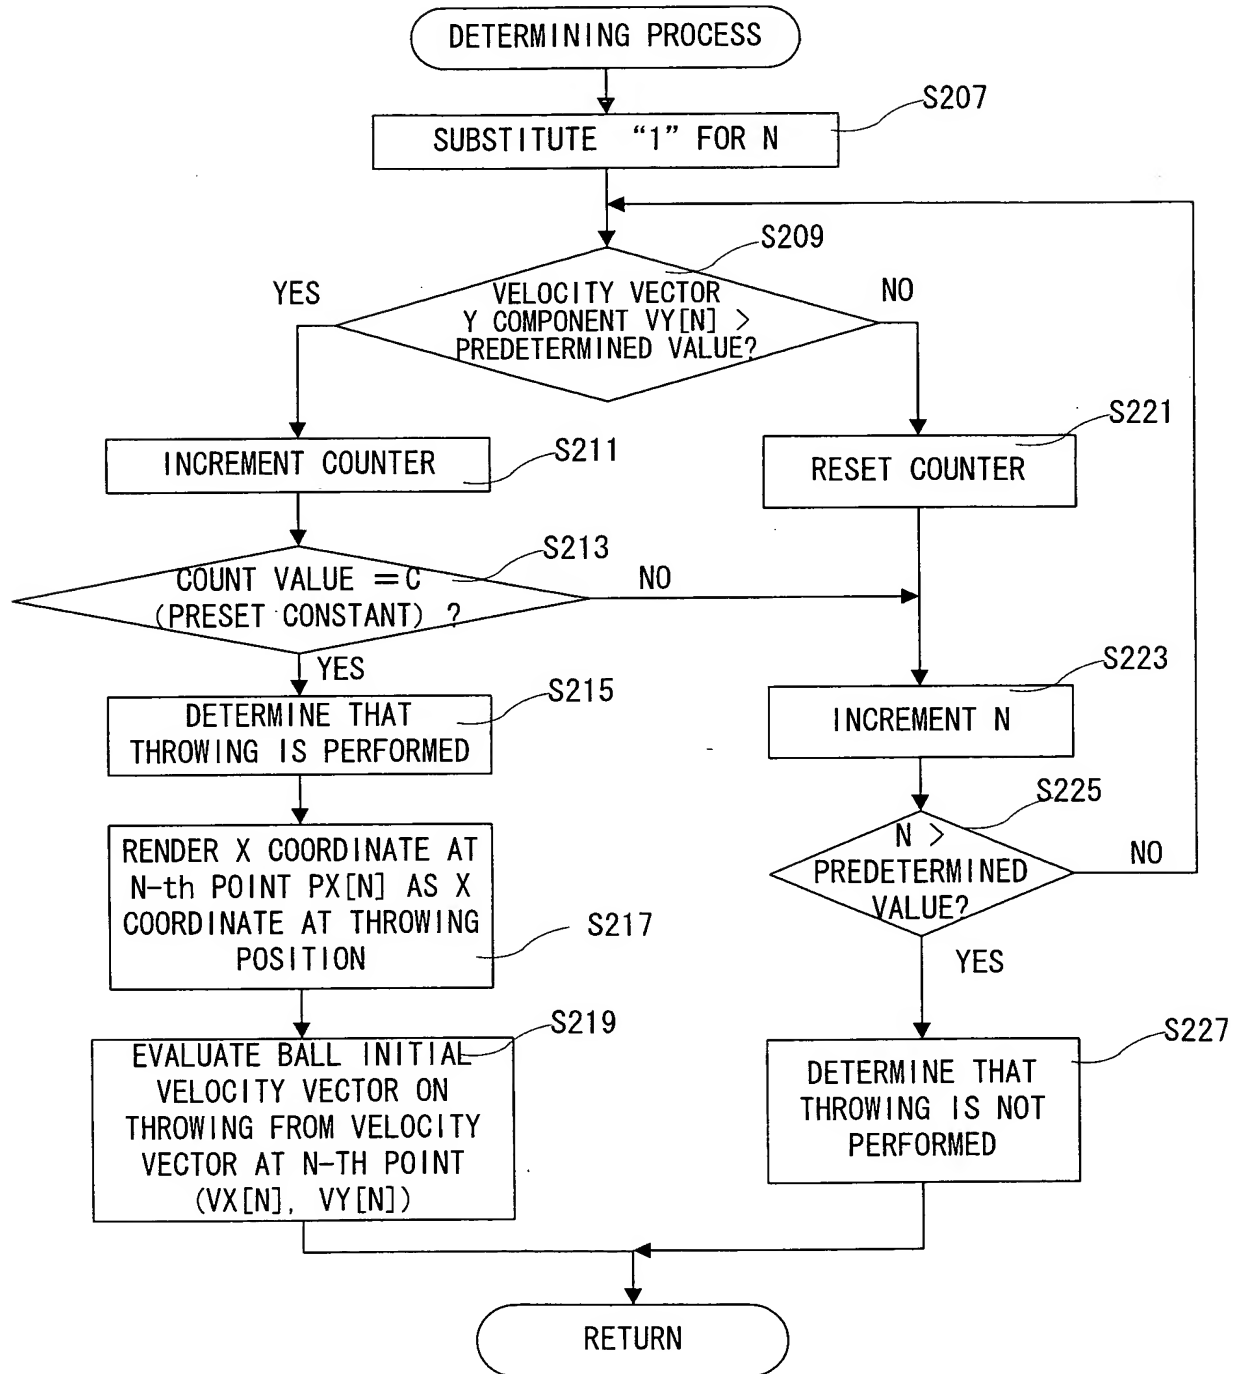


FIG. 34

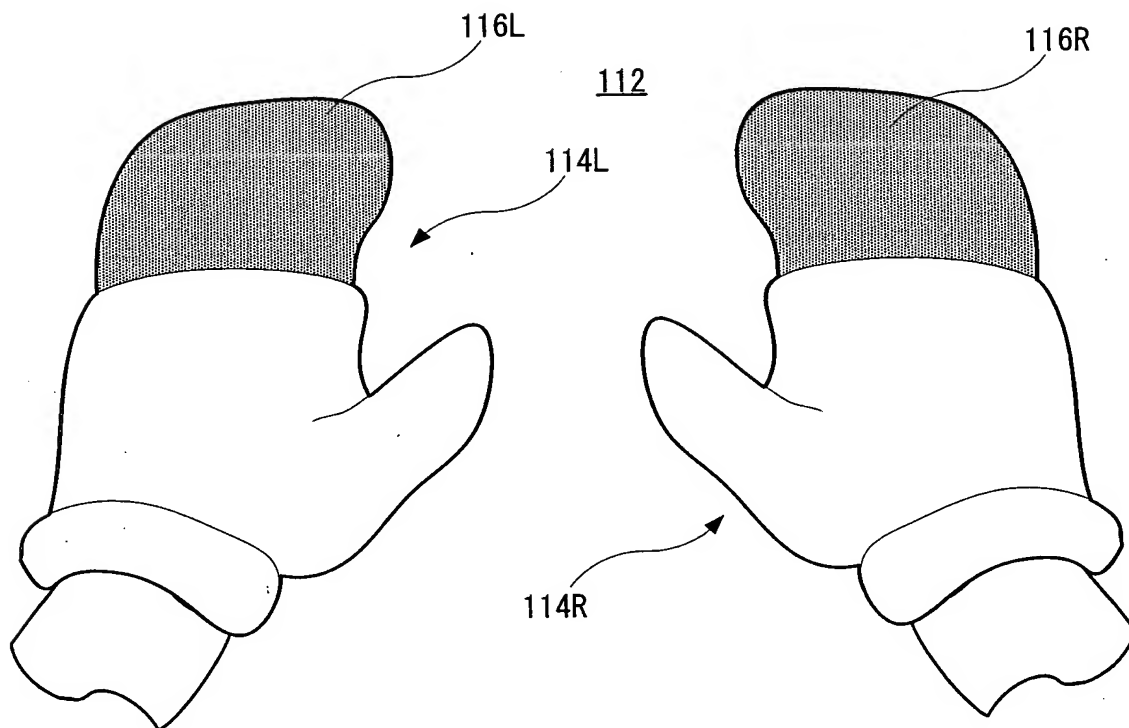


FIG. 35


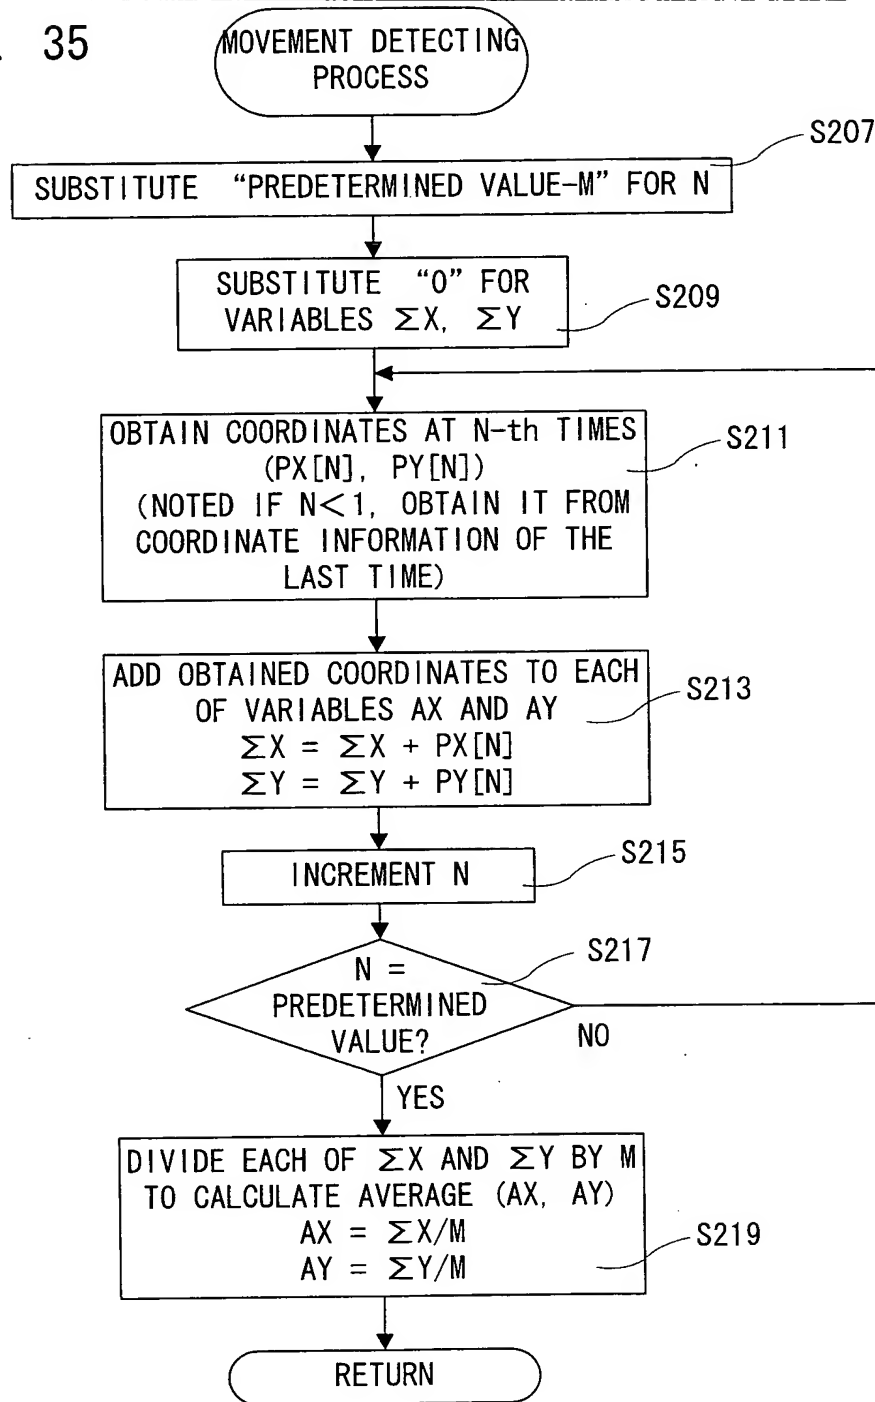


FIG. 36

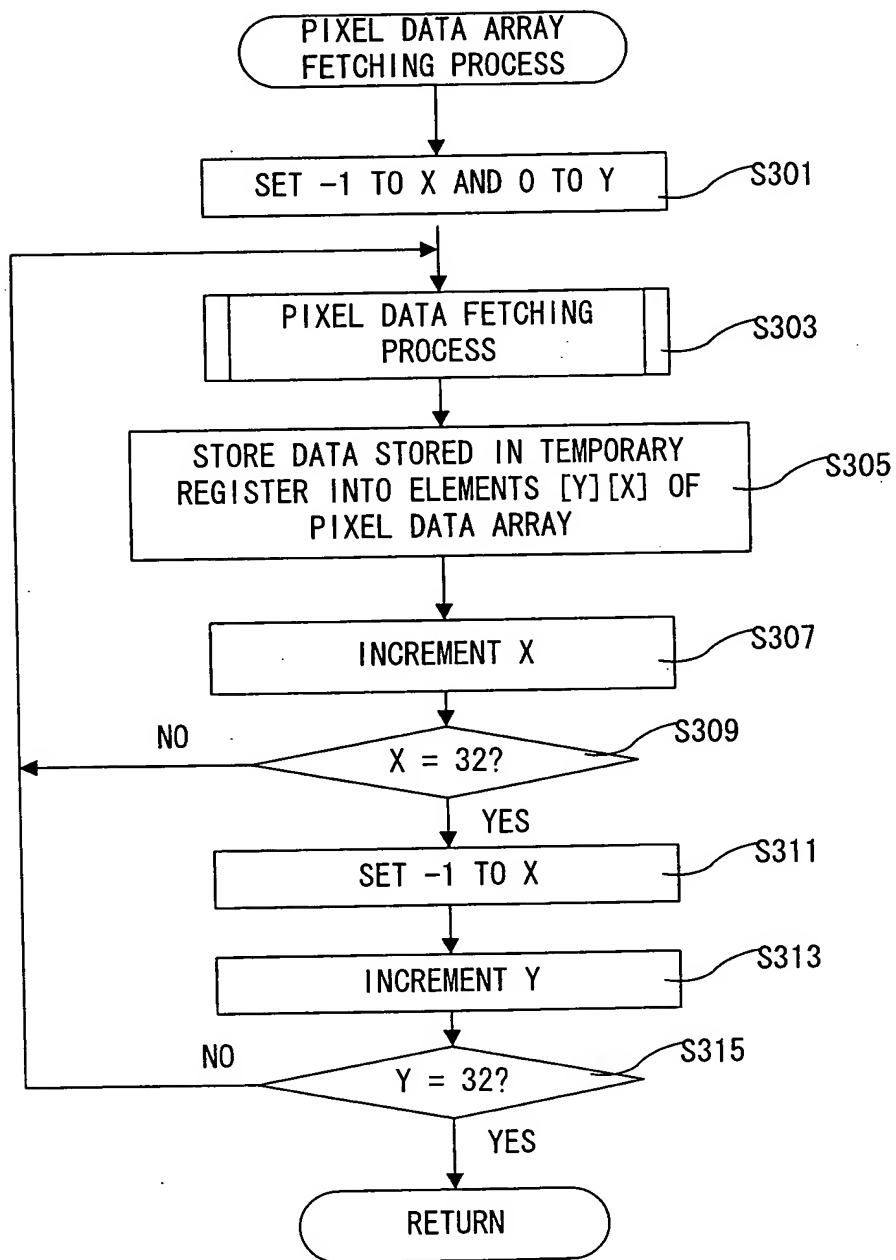

**This Page is Inserted by IFW Indexing and Scanning
Operations and is not part of the Official Record**

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☐ **BLACK BORDERS**
- ☐ **IMAGE CUT OFF AT TOP, BOTTOM OR SIDES**
- ☒ **FADED TEXT OR DRAWING**
- ☒ **BLURRED OR ILLEGIBLE TEXT OR DRAWING**
- ☐ **SKEWED/SLANTED IMAGES**
- ☐ **COLOR OR BLACK AND WHITE PHOTOGRAPHS**
- ☐ **GRAY SCALE DOCUMENTS**
- ☐ **LINES OR MARKS ON ORIGINAL DOCUMENT**
- ☐ **REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY**
- ☐ **OTHER:** _____

IMAGES ARE BEST AVAILABLE COPY.

As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.